




VARIAN
TREATMENT DELIVERY CONSOLE
DICOM CONFORMANCE
STATEMENT

Version 2.0



P1018463-001-A

MAY 2016

Document ID	P1018463-001-A
Document Title	Varian Treatment Delivery Console DICOM Conformance Statement provides information about DICOM conformance with TrueBeam 2.5 MR 2 and 4D Integrated Treatment Console 13.0.
Abstract	The DICOM Conformance Statement provides information about DICOM conformance with TrueBeam 2.5 MR 2 and 4D Integrated Treatment Console 13.0.
Manufacturers	Varian Medical Systems, Inc. 3100 Hansen Way Palo Alto, CA 94304-1038 United States of America
European Authorized Representative	Varian Medical Systems UK Ltd. Oncology House Gatwick Road, Crawley West Sussex RH10 9RG United Kingdom
Notice	Information in this document is subject to change without notice and does not represent a commitment on the part of Varian. Varian is not liable for errors contained in this release note or for incidental or consequential damages in connection with furnishing or use of this material. This document contains proprietary information protected by copyright. No part of this document may be reproduced, translated, or transmitted without the express written permission of Varian Medical Systems, Inc.
FDA 21 CFR 820 Quality System Regulation (cGMPs)	Varian Medical Systems, Oncology Systems products are designed and manufactured in accordance with the requirements specified within this federal regulation.
ISO 13485	Varian Medical Systems, Oncology Systems products are designed and manufactured in accordance with the requirements specified within the ISO 13485 quality standard.
CE	Varian Medical Systems, Oncology Systems products meet the requirements of Council Directive MDD 93/42/EEC.
EU REACH SVHC Disclosure	The link to the current EU REACH SVHC disclosure statement is: http://www.varian.com/us/corporate/legal/reach.html
HIPAA	Varian's products and services are specifically designed to include features that help our customers comply with the Health Insurance Portability and Accountability Act of 1996 (HIPAA). The software application uses a secure login process, requiring a user name and password that supports role-based access. Users are assigned to groups, each with certain access rights, which may include the ability to edit and add data or may limit access to data. When a user adds or modifies data within the database, a record is made that includes which data were changed, the user ID, and the date and time the changes were made. This establishes an audit trail that can be examined by authorized system administrators.
WHO	ICD-O codes and terms used by permission of WHO, from: <ul style="list-style-type: none"> ■ International Classification of Diseases and for Oncology (ICD-O), 3rd edition, Geneva, World Health Organization, 2000. ICD-10 codes and terms used by permission of WHO, from: <ul style="list-style-type: none"> ■ International Statistical Classification of Diseases and Related Health Problems, Tenth Revision (ICD-10). Vols 1–3, Geneva, World Health Organization, 1992.
	CAUTION US Federal law restricts this device to sale by or on the order of a physician.
Trademarks	TrueBeam® is a registered trademark of Varian Medical Systems, Inc. All other trademarks or registered trademarks are the property of their respective owners.

Contents

1. Introduction	5
1.1 Audience	5
1.2 Scope.....	5
1.3 Visual Cues	5
1.4 Contact Varian Customer Support	6
1.5 Definitions.....	7
1.6 Related Documents.....	7
2. Implementation Model.....	8
2.1 Application Data Flow Diagram	8
2.2 Functional Definition of AE's	11
2.3 Sequencing of Real-World Activities	11
3. AE Specifications	13
3.1 Treatment Delivery Console entity Specification	13
3.1.1 Association Establishment Policies.....	13
3.1.2 Association Initiation Policy.....	16
3.1.3 Load and Save of Imager Positions	18
3.1.4 RT Image Position vs. Imager Position in “Planned Verification Image Sequence”.....	19
3.1.5 Primary Fluence Mode	19
3.1.6 Association Acceptance Policy	25
4. Communication profiles.....	28
4.1 Supported communications stacks	28
4.1.1 TCP/IP stack	28
5. Configuration.....	29
5.1 4DITC DICOM Configuration	29
5.1.1 AE Title/Presentation Address Mapping	29
5.1.2 Configurable Parameters	29
5.2 TxA DICOM Configuration	30
6. Media Interchange.....	31
7. Support of Extended Character Sets	31
8. Security	31
8.1 Security Profiles	31
8.2 Association Level Security	31
8.3 Application Level Security	31

Appendix A	Specialization	32
A.1	IOD Contents	32
A.1.1	Created SOP Instances	32
A.1.2	Usage of Attributes from received IOD's	32
A.2	Data Dictionary of Private Attributes	34
A.2.1	Privatization for RT Plan Storage SOP class	34
A.2.2	Privatization for RT Beams Treatment Record Storage SOP class	36
A.2.3	Privatization for RT Treatment Summary Record Storage SOP class	37
Appendix B	DICOM Query Retrieve Service Class Object Matching Criteria (SCU Role)	38
B.1	IOD Specific Matching Criteria	38
B.1.1	Supported Keys	39
Appendix C	IOD Details	42
C.1	Supported IODs	42
C.2	Modules and Attributes	45
C.2.1	Patient – C.7.1.1	45
C.2.2	General Study - C.7.2.1	47
C.2.3	Frame of Reference – C.7.4.1	53
C.2.4	General Equipment – C.7.5.1	54
C.2.5	RT Series – C.8.8.1	55
C.2.6	RT General Plan – C.8.8.9	63
C.2.7	RT Prescription – C.8.8.10	65
C.2.8	RT Tolerance Tables – C.8.8.11	68
C.2.9	RT Patient Setup – C.8.8.12	71
C.2.10	RT Fraction Scheme – C.8.8.13	75
C.2.11	RT Beams – C.8.8.14	80
C.2.12	Approval – C.8.8.16	106
C.2.13	SOP Common – C.12.1	107
C.2.14	Extended Interface – Private	116
Appendix D	Extended Interface	117
D.1	RT Plan	117
D.2	RT Beams Treatment Record	120

1. Introduction

The definition of the DICOM standard for radiotherapy data started in 1994, and has now reached a productive state. Today, DICOM is the primary choice for exchanging data with an open standard protocol for the majority of vendors and institutions. Varian Medical Systems is committed to this notion and supports the full range of radiotherapy objects (e.g. RT Plan, RT Image, RT Beams Treatment Record) for their V & R system.

This conformance statement specifies the conformance of the **TrueBeam TxA console version 2.5 MR 2** and **4D Integrated Treatment Console version 13.0** with the DICOM V 3.0 standard.

1.1 Audience

This document is intended for the following groups of persons:

- Marketing and Sales.
- System Integrators of medical equipment.
- Other vendors interfacing via DICOM

It is assumed that the reader is familiar with the DICOM standard.

1.2 Scope

This Conformance Statement is applicable to the following Varian treatment delivery consoles:

- TrueBeam TxA version 2.5 MR 2
- 4D Console version 13.0.

The general DICOM conformance statement for Varian Medical Systems products is defined in [2] (see section 1.7).

This Conformance Statement describes only the specials and the variations as implemented in TrueBeam TxA version 2.5 MR2 and 4D Integrated Treatment Console version 13.0

The scope and format of this document are defined by Part 2 of the DICOM V3.0 standard. Some sections defined in the standard that are not applicable to the software are left out for clarity.

1.3 Visual Cues

This document uses the following visual cues to help you locate and find information:



Note A note describes practices not related to physical injury.



CAUTION A caution describes a hazardous situation which, if not avoided, could result in minor or moderate injury.



WARNING A warning describes a hazardous situation which, if not avoided, could result in death or serious injury.

1.4 Contact Varian Customer Support

Varian Customer Support is available on the internet, by e-mail, and by telephone. Support services are available without charge during the initial warranty period.

The MyVarian website provides contact information, product documentation, and other resources for all Varian products.

1. Go to www.MyVarian.com.
2. Choose an option:
 - If you have an account, enter your User login information (email and password).
 - If you do not have an account, click **Create New Account** and follow the instructions. Establishing an account may take up to two working days.
3. Click **Contact Us** at the top of the window to display customer support and training options, and international e-mail addresses and telephone numbers.
4. From the Contact Us page, choose an option:
 - Call Varian Medical Systems support using a phone support number for your geographic area.
 - Complete the form corresponding to your request for use on a call with a live Varian representative; then follow the instructions to complete the remote connect options, and click **Submit**.

You can order documents by phone, request product or applications support, and report product-related issues. Links on the MyVarian website navigate to other support resources for products, services, and education.

5. To find documents, click **Product Documentation**.
Online documents in PDF format include customer technical bulletins (CTBs,) manuals, and customer release notes (CRNs).

1.5 Definitions

This section provides the definitions of terms, acronyms, and abbreviations, which are used throughout the document.

4DITC	4D Integrated Treatment Console
AE	Application Entity
DB	Database
DICOM	Digital Imaging and Communications in Medicine
DIMSE	DICOM Message Service element
DNS	Domain Name System
EMPTY	Attribute is sent without a value
IOD	Information Object Definition
Management System	DICOM entity from which TREATMENT DELIVERY retrieves patient data
Multi-Frame Image	Image that contains multiple two-dimensional pixel planes
NEMA	National Electrical Manufacturers Association
PDU	Protocol Data Unit (a DICOM term)
PVA	Patient Verification Application (a TrueBeam Imaging Application)
SCU	Service Class User
SCP	Service Class Provider
SOP	Service Object Pair
TCP/IP	Transmission Control Protocol / Internet Protocol
TXA	TrueBeam Treatment Application
VNAP	Value Not Always Present (attribute sent zero length if no value is present)
VR	Value Representation

1.6 Related Documents

- Digital Imaging and Communications in Medicine (DICOM), Parts 1-18 (2008), National Electrical Manufacturers Association (NEMA) Rosslyn, Virginia, United States of America
- Varian System Server DICOM Conformance Statement B VA8005D3DCS Baden, Switzerland

2. Implementation Model

Three diagrams illustrating the application model, two for the SCU and one for the SCP role, are shown in Figure 1, Figure 2, and Figure 3.

2.1 Application Data Flow Diagram

The initial function to load the plan into the treatment delivery console application is represented by *Load RT Plan* (This function is typically performed by the application after the Patient and the Plan UIDs have been received by the Management System). The treatment delivery console invokes a move command for each DICOM RT Plan. This requires the treatment delivery console application to provide the RT Plan Storage SCP. Figure 2 shows the Service Class Providers (SCP) role supported by the treatment delivery console. The treatment delivery console then issues a move command to request and retrieve the RT Treatment Summary Record. Based on the last fraction state, a find command is executed to request the *Load Beam Record Information* (shown in Figure 1) to recover from a partial treatment.

A *Save* issued by the operator will invoke a storage command, which requires the remote application to provide a storage SCP as shown in Figure 3.

Closing the patient in the treatment delivery console will result in a *Save* if the plan data has been modified and/or treatment records and images have been created. The treatment delivery console will delete the objects temporarily stored. In case the Management System is not accessible, The treatment delivery console will save the changes into one or several DICOM Media files.

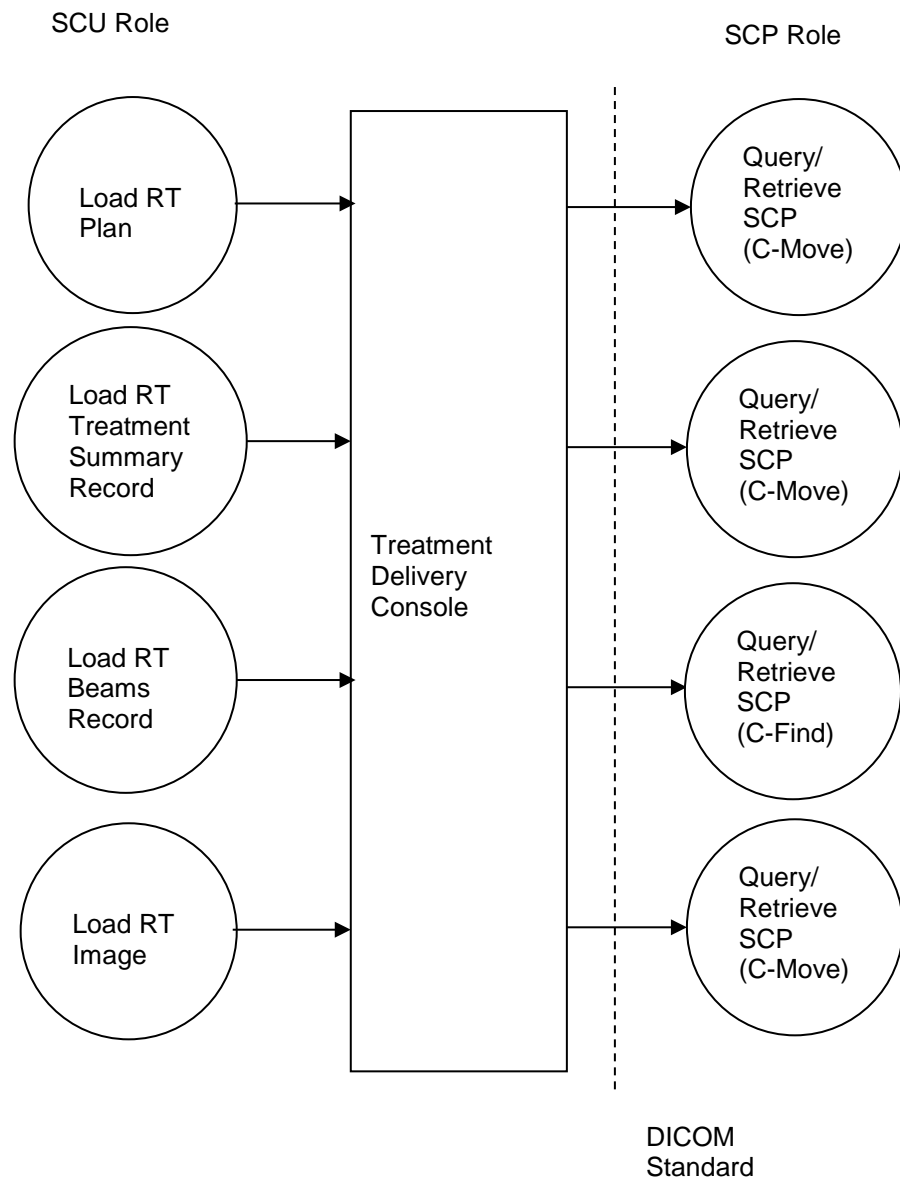


Figure 1: SCU Role Application Data Flow Diagram for Loading Patient Data

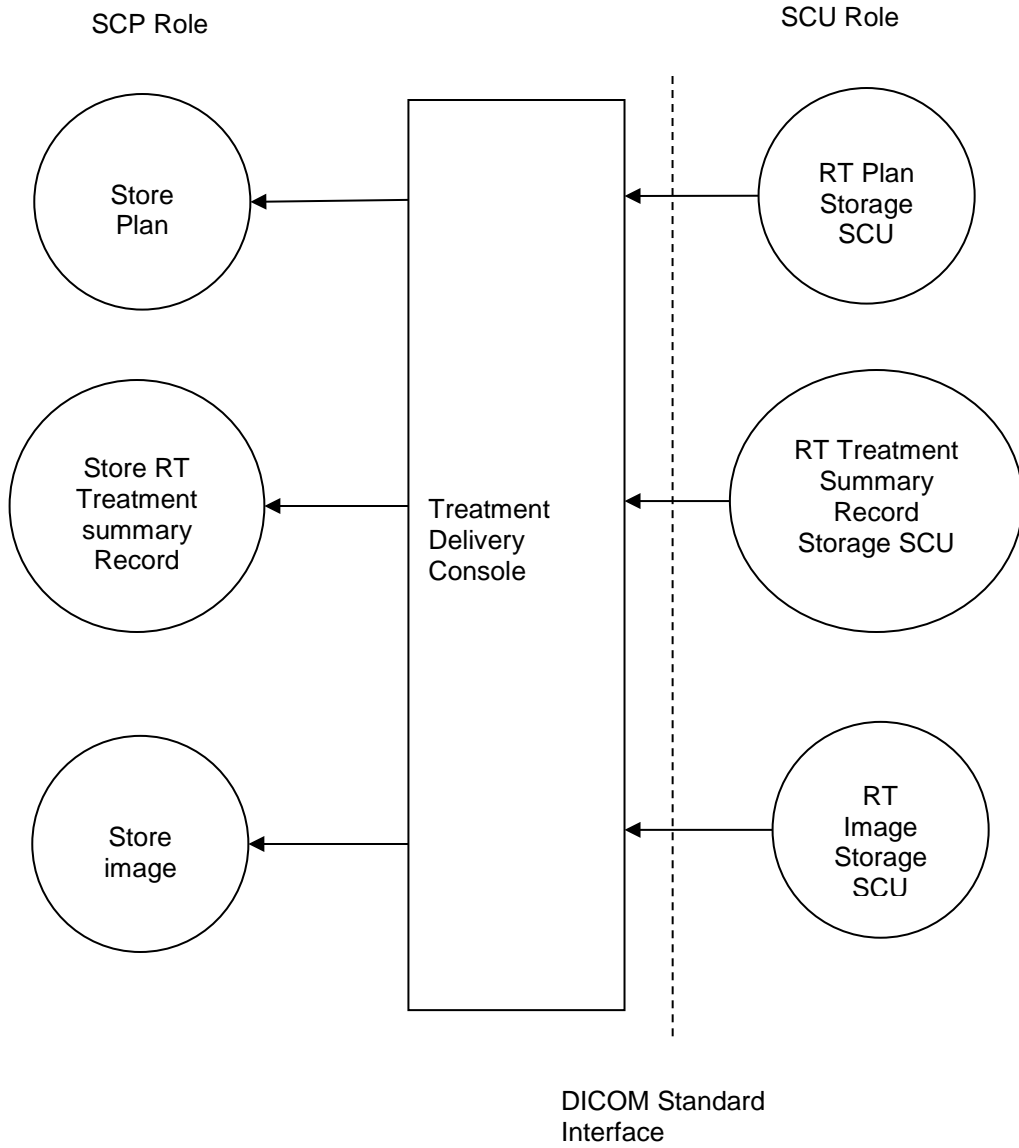


Figure 2: SCP Role Application Data Flow Diagram for Loading Patient Data

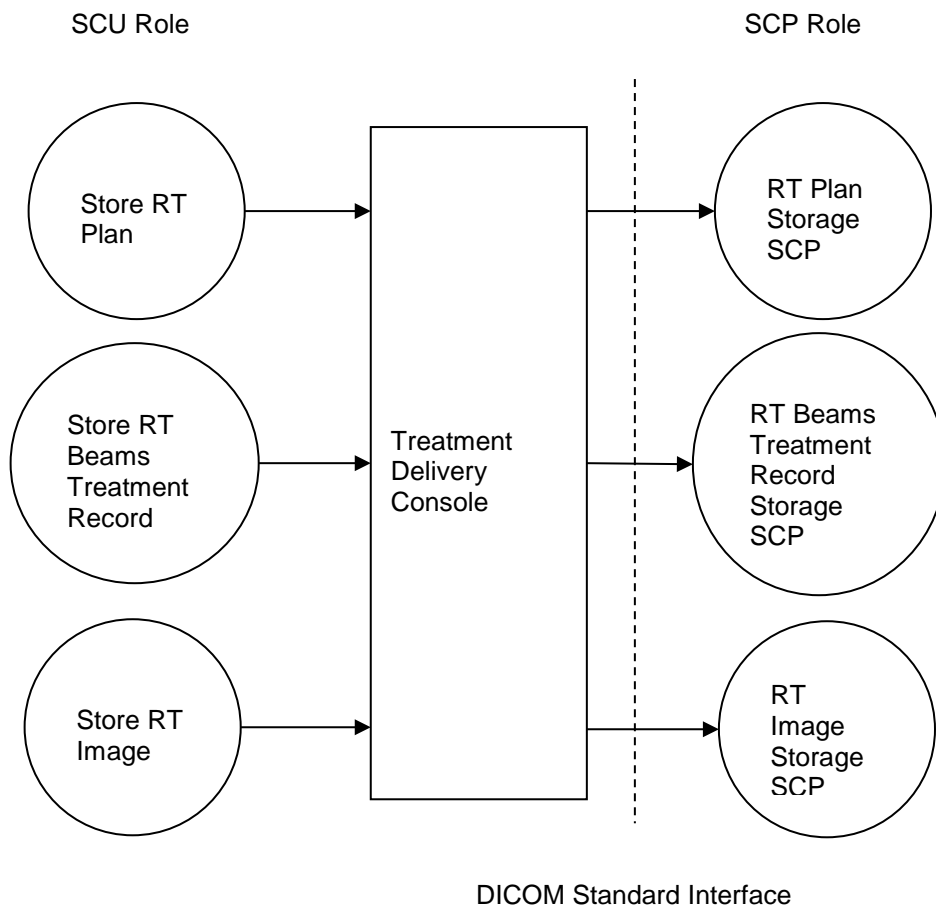


Figure 3: SCU Role Application Data Flow Diagram for Saving Patient Data

2.2 Functional Definition of AE's

The treatment delivery console entity's main responsibility is to execute a patient treatment. Before treating, the treatment delivery console loads the patient data from the Management System using DICOM services. After treating, the treatment delivery console generates RT Beams Treatment Record(s) and RT Image(s). The treatment delivery console then stores them back to the Management System again using DICOM services.

The treatment delivery console is also capable of modifying RT Plan(s) and/or creating new RT Plan(s).

2.3 Sequencing of Real-World Activities

The treatment delivery console executes the activities for loading a patient in the following order.

1. C-Find RT Plan SOP class (see section 3.1.2.2.3.2).
2. C-Move RT Plan SOP class.
3. C-Move RT Treatment Summary Record SOP class.
4. C-Find RT Beams Treatment Record SOP class if needed.



No *C-Find RT Beams Treatment Record query is only executed in order to*
te *finalize the previous treated fraction.*

The 4DITC console also retrieves referenced RT Images. The steps below only apply to the 4DITC console.

5. C-Move RT Image SOP class (for Reference Images if referred in the RT Plan)
6. C-Find RT Image SOP class (for query Portal Images).
7. C-Move RT Image SOP class (for Portal Images if query returned Portal Image Instance [UIDs]).

The only requirement is to load the RT Plan first before the others. This sequence may be performed for more than one plan at the beginning of a treatment session.

The patient record is saved in the following order to treatment delivery console:

1. C-Store RT Plan SOP class (executed if a plan is changed in treatment delivery console).
2. C-Store RT Beams Treatment Record SOP class (executed if a beam was treated).
3. C-Store RT Image SOP class (executed if a Portal Image was acquired) (4DITC only).

The only requirement is to save RT Plans first before the RT Beam Records and RT Images. This is because the RT Beams Treatment Record and/or RT Image may refer to the new RT Plan.

3. AE Specifications

3.1 Treatment Delivery Console entity Specification

The treatment delivery console entity provides standard conformance to the following DICOM V3.0 SOP classes:

SOP Class Name	SCU/SCP Role	SOP Class UID
Verification (Echo)	SCU / SCP	1.2.840.10008.1.1
RT Image Storage	SCU / SCP	1.2.840.10008.5.1.4.1.1.481.1
RT Plan Storage	SCU / SCP	1.2.840.10008.5.1.4.1.1.481.5
RT Treatment Summary Record Storage	SCP	1.2.840.10008.5.1.4.1.1.481.7
Study Root Query/Retrieve information model- FIND	SCU	1.2.840.10008.5.1.4.1.2.2.1
Study Root Query/Retrieve information model- MOVE	SCU	1.2.840.10008.5.1.4.1.2.2.2
RT Beams Treatment Record Storage	SCU	1.2.840.10008.5.1.4.1.1.481.4

Table 1: Supported SCU/SCP SOP Classes for the Treatment Delivery Console Entity

3.1.1 Association Establishment Policies

3.1.1.1 General

See details in Related Documents.

There are a total of three associations. The treatment delivery console establishes two associations while the Management System establishes one association. The first association established by treatment delivery console is to support the C-Move and C-Find services. The second association established by treatment delivery console is to support the C-Store service. The association established by the Management System is for storing patient data to treatment delivery console.

All of the association supports the C-Echo service to determine whether the association is still alive or not.

A diagram of the associations is in Figure 4.

4DITC accepts any maximum PDU size for incoming data streams and suggests the size of 65536 for outgoing data streams.

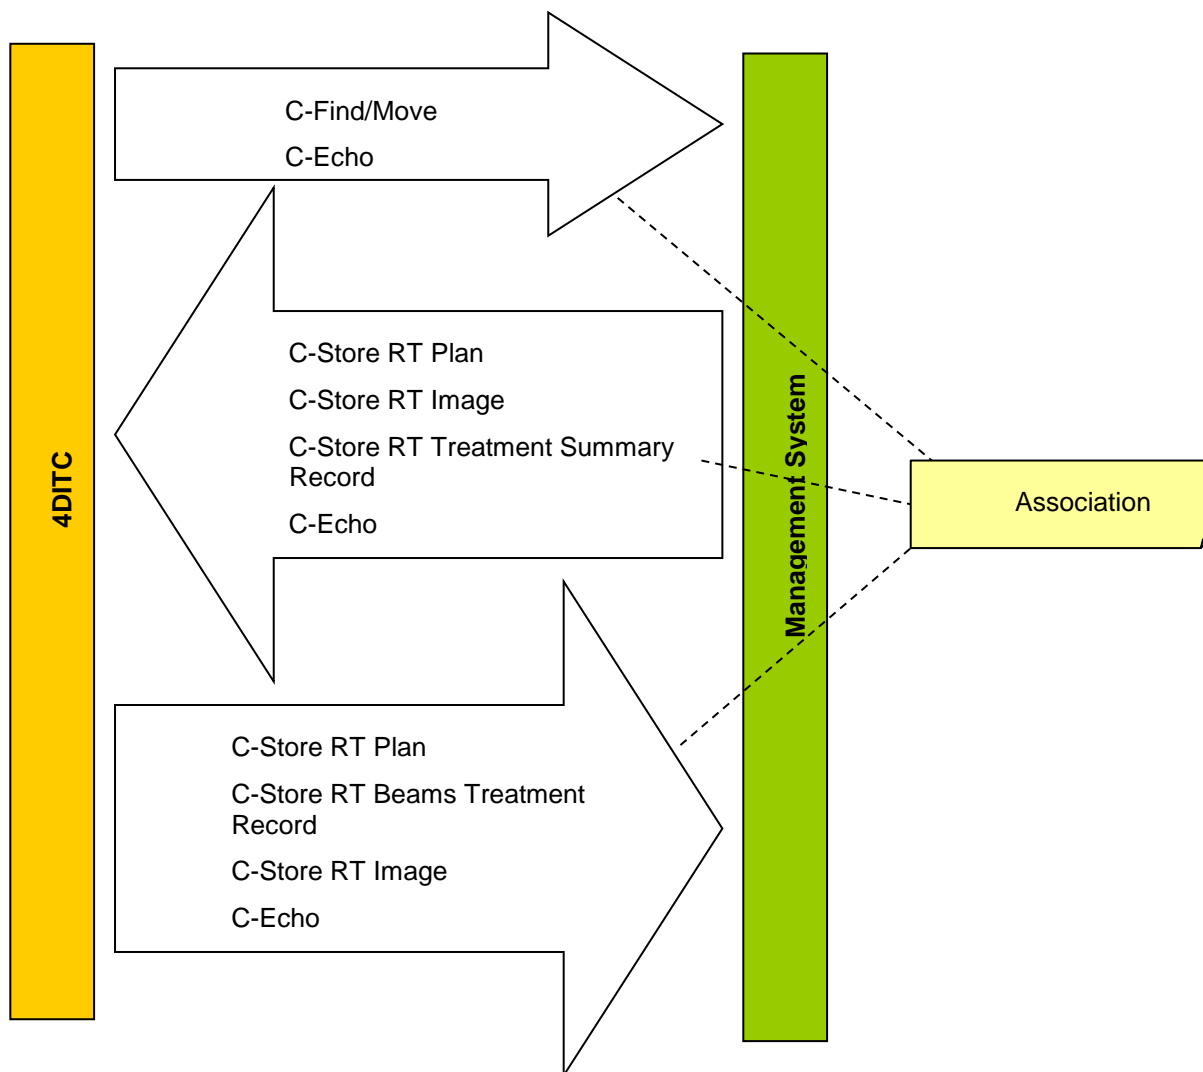


Figure 4: Associations Used for 4DITC

3.1.1.2 Number of Associations

The treatment delivery consoles support a total of three associations as shown in Figure 4. They support having one association for each batch of services at a time.

A batch of services refers to the list of services contained in an arrow in Figure 4.

3.1.1.3 Asynchronous Nature

Asynchronous operation is not supported.

3.1.1.4 Implementation identifying information

UID Value	UID Name	Notes
1.2.246.352.70.2.1.9	VMS Console System 6.5 SCU (VMS Console Interface 1)	TrueBeam and 4DITC
1.2.246.352.70.2.1.10	VMS Console System 6.5 SCP	—
1.2.246.352.70.2.1.17	VMS Console Interface 3	4DITC 8.8 and higher
1.2.246.352.70.2.1.18	VMS Console System 8.8 SCP	Treatment Daemon 8.8
1.2.246.352.70.2.1.19	VMS Console Interface 3 QA Mode	4DITC 8.8 (for QA Mode) and higher
1.2.246.352.70.2.1.20	VMS Console System 8.8 QA Mode SCP	Treatment Daemon 8.8
1.2.246.352.70.2.1.81.4.1	VMS Console Interface 4	4DITC 10 and higher
1.2.246.352.70.2.1.82.4.1	VMS Treatment Daemon 10.0 SCP	Treatment Daemon 10.0
1.2.246.352.70.2.1.81.4.2	VMS Console Interface 4 QA Mode	4DITC 10.0 (for QA Mode) and higher
1.2.246.352.70.2.1.82.4.2	VMS Treatment Daemon 10.0 QA Mode SCP	Treatment Daemon 10.0
1.2.246.352.70.2.1.81.5.1	VMS Console Interface 5	4DITC 11 and higher
1.2.246.352.70.2.1.82.5.1	VMS Treatment Daemon 11.0 SCP	Treatment Daemon 11
1.2.246.352.70.2.1.81.5.2	VMS Console Interface 5 QA Mode	4DITC 11 (for QA Mode) and higher
1.2.246.352.70.2.1.82.5.2	VMS Treatment Daemon 11.0 QA Mode SCP	Treatment Daemon 11
1.2.246.352.70.2.1.81.6.1	VMS Console Interface 6	4DITC 13 and higher
1.2.246.352.70.2.1.81.6.2	VMS Treatment Daemon 13.0 SCP	Treatment Daemon 13
1.2.246.352.70.2.1.82.6.1	VMS Console Interface 6 QA Mode	4DITC 13 (for QA Mode) and higher
1.2.246.352.70.2.1.82.6.2	VMS Treatment Daemon 13.0 SCP	Treatment Daemon 13

Table 2: 4DITC List of implementation UIDs and application support

1.2.246.352.70.2.1.9	VMS Console System 6.5 SCU (VMS Console Interface 1)	—
1.2.246.352.70.2.1.10	VMS Console System 6.5 SCP	—
1.2.246.352.70.2.1.17	VMS Console Interface 3	—
1.2.246.352.70.2.1.18	VMS Console System 8.8 SCP	—
1.2.246.352.70.2.1.19	VMS Console Interface 3 QA Mode	—
1.2.246.352.70.2.1.20	VMS Console System 8.8 QA Mode SCP	—

Table 3: TrueBeam TxA list of implementation UIDs supported and used

3.1.2 Association Initiation Policy

The treatment delivery console entity will initiate one association for all Query/Retrieve Services (Q/R SCU) that contains the C-Find and the C-Move service. When the user starts up 4DITC and clicks on "Open Patient", 4DITC initiates an association for all Query/Retrieve Services for the first time.

The 4DITC Entity will initiate one association for all Storage Services where it acts as a user (Storage SCU). When the user clicks "Save Images" ("Save images" is applicable to 4DITC only) or "Close Patient", 4DITC checks if an association already exists for all Storage Services. If an association does not exist for all Storage Services, 4DITC initiates an association for all Storage Services. Otherwise, 4DITC uses the existing association.

The Management System will initiate one association for all C-Store services used for sending all patient data. In this association, 4DITC acts as a provider (Storage SCP).

The Echo/Verification service is used prior to any other DICOM service to verify whether an established association exists.

3.1.2.1 Storage SCU

3.1.2.1.1 Associated Real-World Activity

The C-Store service is used by 4DITC to store patient data into the Management System. This service gets executed whenever the operator selects 'Close Patient' or 'Save Image'.

3.1.2.1.2 Presentation Context Table

Presentation Context Table							
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation	TxA 2.5	4DITC 13.0
Name	UID	Name	UID				
RT Plan Storage	1.2.840.10008.5.1.4.1.1.481.5	DICOM Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None	Yes	Yes
RT Beams Treatment Record Storage	1.2.840.10008.5.1.4.1.1.481.4	DICOM Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None	Yes	Yes
RT Image Storage	1.2.840.10008.5.1.4.1.1.481.1	DICOM Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None	Yes	Yes

Table 4: Proposed Presentation Contexts for Storage SCU

3.1.2.1.3 SOP Specific Conformance

3.1.2.1.3.1 SOP Specific Conformance for All Storage SOP Classes

After a successful C-STORE operation, the treatment delivery console does not display any information to the user but returns to its normal state. If the C-STORE operation results with a warning or an error, the treatment delivery console displays the appropriate warning or error message to the operator.

3.1.2.1.3.2 SOP Specific Conformance for the RT Plan Storage SOP Class

3.1.2.1.3.2.1 4DITC (only) with implementation UID 'Varian Console Interface 4' and 'Varian Console Interface 4 QA Mode' or later

These tags are in addition to conformance rules applied for lower version of implementation UIDs supported in older version of Varian treatment delivery console.

Varian treatment delivery consoles use the following tags from 'Patient Setup Sequence (300A, 0180):

- Table Top Vertical Setup Displacement (300A, 01d2).
- Table Top Longitudinal Setup Displacement (300A, 01d4).
- Table Top Lateral Setup Displacement (300A, 01d6).

Also, when SOP object has at least one table top setup displacement defined, 4DITC (only) considers zero value for remaining undefined table top setup displacements.



No Table top displacement values listed above are not supported by
te TrueBeam v2.5

3.1.2.1.3.2.2 Varian treatment delivery consoles communicating on implementation UID "Varian Console Interface 3" and "Varian Console Interface 3 QA Mode" or later:

These tags are in addition to conformance rules applied for lower version of implementation UIDs supported in older version of 4DITC.

- Treatment Delivery Type (300A, 00CE) supports new defined Term SETUP attribute for Setup Fields.
- Accessory Code (300A, 00F9) for Wedge, Compensator, Block and Applicator.
- Varian treatment delivery consoles do not accept Arc-Dynamic Beam(s), which contain gantry rotations that are not equally spaced (e.g. 0, 10, 30, 100).
- Only the first Fraction Group sequence (300A, 0070) is read. The others are discarded.
- A maximum of two wedges per field are supported.
- A maximum of one MLC per field is supported.
- Beam energy, table parameter and rotation direction changes in the control points are not supported.
- Whenever an operator changes a dose relevant attribute from the RT Plan in 4DITC, a new RT Plan is created. The new RT Plan will refer to the originally loaded RT Plan through the Referenced RT Plan Sequence (300C, 0002). The Referenced RT Plan Sequence (300C, 0002) can only contain at most one item.
- General Accessory Sequence (300A,0420) used for empty Trays.

RT Plan extended interface and privatization are described in section 4.

Replacement for Field Type

In Extended Interface FieldType is used to distinguish between treatment and setup fields (values: TREATMENT, SETUP) while DICOM attribute Treatment Delivery Type (300A, 00CE) always contains value TREATMENT. When FieldType is removed from Extended Interface, the new value SETUP for Treatment Delivery Type (300A,00CE) is used to designate setup fields.

Replacement for CustomAddOn for Block and Compensator

For Block and Compensator the Extended Interface has been used only to transport the accessory code. This has been added to the DICOM standard and is now available in various accessory sequences as attribute Accessory Code (300A,00F9), RT Beams Module.

- Compensator Sequence (300A,00E3): Accessory Code (300A,00F9).
- Block Sequence (300A, 00F4): Accessory Code (300A,00F9)

Replacement for CustomAddOn for Empty Trays

Empty trays are trays that are not used for mounting a block or compensator but for different purposes not supported specifically by DICOM. With the introduction of the General Accessory Sequence (300A,0420) in RT Beams Module the CustomAddOn attribute in Extended Interface gets obsolete for empty trays.

Empty Trays in General Accessory Sequence

General Accessory Sequence (300A,0420):

- General Accessory Number (300A,0424)
- General Accessory ID (300A,0421) – Replaces TrayID
- General Accessory Description (300A,0422) –
- General Accessory Type (300A,0423) – Defined Term: TRAY
- Accessory Code (300A,00F9) – Replaces CustomCode

Bolus Support

- Number of Boli (300A, 00ED) in Beam Sequence (300A, 00B0) is used for manual verification.
- Referenced ROI number (3006, 0084) is used to identify the bolus is same or different within a plan.

3.1.3 Load and Save of Imager Positions

It is possible to transfer the imager positions between the management system and 4DITC Applications even if no verification images are planned or taken and thus “Planned Verification Image Sequence” (300A,00CA) in RT Beams Module is empty.

If the “Planned Verification Image Sequence” is empty, a pseudo verification image will be added to this sequence whose only purpose is to transmit the imager positions. This is done by adding an item to this sequence containing only the following attributes:

- X-Ray Image Receptor Angle (3002,000E)
- RT Image Position (3002,0012)
- RT Image SID (3002,0026)
- Imaging Device-Specific Acquisition Parameters (300A,00CC) containing the string “Default Imaging Parameters”

When 4DITC Application sends back a plan to the management System it may omit the tag “X-Ray Image Receptor Angle” (3002,000E) because this value must be 0.0 (zero) anyway.

When imager positions are changed on 4DITC Application they will be saved back to the management system when closing the patient. Management system saves imager positions that are listed in the “Planned Verification Image Sequence” for sending them again to 4DITC Application when the plan is requested next time.

3.1.4 RT Image Position vs. Imager Position in “Planned Verification Image Sequence”

The DICOM standard defines the “RT Image Position” (3002,0012) as “The x and y coordinates [...] of the upper left hand corner [...] of the image [...]”.

Because the size of an image to be taken is not known in advance, a width and height of zero pixels is assumed in the “Planned Verification Image Sequence” of an RT Plan IOD. Therefore the position of the center of the image receptor will be used for the “RT Image Position” tag instead. This is because these are the same coordinates as those of the upper left hand corner of an image with zero pixels in x and y directions.

- The treatment delivery consoles will only accept the Beam Limiting Device if the verification of the treatment machine settings and the Beam Limiting Device were successful. The same rule applies to the imported Wedge, Block and Applicator data.
- The treatment delivery console does not accept Arc-Dynamic Beam(s), which contains gantry rotations that is not equally spaced (e.g. 0, 10, 30, and 100).
- Only the first Fraction Group sequence (300A, 0070) is read. The others are discarded.
- A maximum of two wedges per field are supported.
- A maximum of one MLC per field is supported.
- Beam energy, table parameter and rotation direction changes in the control points are not supported.
- Wedge position changes are only supported for static technique (motorized wedge).

3.1.5 Primary Fluence Mode

3.1.5.1 TrueBeam TxA

The supported combination of High dose technique, Dose rate, Primary fluence mode and energy are listed in Table 3.

Nominal Beam Energy (MV/MeV) (300A,0114)	Dose Rate Set MU/Min (300A, 0115)	Primary Fluence Mode (3002,0051)*	High-Dose Technique Type (300A,00C7)
2.5x	60	<input checked="" type="checkbox"/> STANDARD <input type="checkbox"/> NON_STANDARD	<input type="checkbox"/> Normal <input type="checkbox"/> TBI <input type="checkbox"/> HDR <input type="checkbox"/> SRS
4x	5, 10, 15, 20, 30, 40, 50, 100, 150, 200, 250	<input checked="" type="checkbox"/> STANDARD <input type="checkbox"/> NON_STANDARD	<input checked="" type="checkbox"/> Normal <input checked="" type="checkbox"/> TBI <input type="checkbox"/> HDR <input checked="" type="checkbox"/> SRS
6x	5, 10, 15, 20, 40, 60, 80, 100, 200, 300, 400, 500, 600	<input checked="" type="checkbox"/> STANDARD <input type="checkbox"/> NON_STANDARD	<input checked="" type="checkbox"/> Normal <input checked="" type="checkbox"/> TBI <input type="checkbox"/> HDR <input checked="" type="checkbox"/> SRS
6x FFF	400, 600, 800, 1000, 1200, 1400	<input type="checkbox"/> STANDARD <input checked="" type="checkbox"/> NON_STANDARD	<input checked="" type="checkbox"/> Normal <input checked="" type="checkbox"/> TBI <input type="checkbox"/> HDR <input checked="" type="checkbox"/> SRS

8x	5, 10, 15, 20, 40, 60, 80, 100, 200, 300, 400, 500, 600	<input checked="" type="checkbox"/> STANDARD <input type="checkbox"/> NON_STANDARD	<input checked="" type="checkbox"/> Normal <input checked="" type="checkbox"/> TBI <input type="checkbox"/> HDR <input checked="" type="checkbox"/> SRS
10x	5, 10, 15, 20, 40, 60, 80, 100, 200, 300, 400, 500, 600	<input checked="" type="checkbox"/> STANDARD <input type="checkbox"/> NON_STANDARD	<input checked="" type="checkbox"/> Normal <input checked="" type="checkbox"/> TBI <input type="checkbox"/> HDR <input checked="" type="checkbox"/> SRS
10x FFF	400, 600, 800, 1000, 1200, 1400, 2400	<input type="checkbox"/> STANDARD <input checked="" type="checkbox"/> NON_STANDARD	<input checked="" type="checkbox"/> Normal <input checked="" type="checkbox"/> TBI <input type="checkbox"/> HDR <input checked="" type="checkbox"/> SRS
15x	20, 40, 60, 80, 100, 200, 300, 400, 500, 600	<input checked="" type="checkbox"/> STANDARD <input type="checkbox"/> NON_STANDARD	<input checked="" type="checkbox"/> Normal <input checked="" type="checkbox"/> TBI <input type="checkbox"/> HDR <input checked="" type="checkbox"/> SRS
18x	20, 40, 60, 80, 100, 200, 300, 400, 500, 600	<input checked="" type="checkbox"/> STANDARD <input type="checkbox"/> NON_STANDARD	<input checked="" type="checkbox"/> Normal <input checked="" type="checkbox"/> TBI <input type="checkbox"/> HDR <input checked="" type="checkbox"/> SRS
20x	20, 40, 60, 80, 100, 200, 300, 400, 500, 600	<input checked="" type="checkbox"/> STANDARD <input type="checkbox"/> NON_STANDARD	<input checked="" type="checkbox"/> Normal <input checked="" type="checkbox"/> TBI <input type="checkbox"/> HDR <input checked="" type="checkbox"/> SRS
4e	100, 200, 300, 400, 500, 600, 700, 800, 900, 1000	<input checked="" type="checkbox"/> STANDARD <input type="checkbox"/> NON_STANDARD	<input checked="" type="checkbox"/> Normal <input checked="" type="checkbox"/> TBI <input type="checkbox"/> HDR <input type="checkbox"/> SRS
6e	100, 200, 300, 400, 500, 600, 700, 800, 900, 1000 2500 for HDR	<input checked="" type="checkbox"/> STANDARD <input type="checkbox"/> NON_STANDARD	<input checked="" type="checkbox"/> Normal <input checked="" type="checkbox"/> TBI <input checked="" type="checkbox"/> HDR <input type="checkbox"/> SRS
9e	100, 200, 300, 400, 500, 600, 700, 800, 900, 1000 2500 for HDR	<input checked="" type="checkbox"/> STANDARD <input type="checkbox"/> NON_STANDARD	<input checked="" type="checkbox"/> Normal <input checked="" type="checkbox"/> TBI <input checked="" type="checkbox"/> HDR <input type="checkbox"/> SRS
12e	100, 200, 300, 400, 500, 600, 700, 800, 900, 1000	<input checked="" type="checkbox"/> STANDARD <input type="checkbox"/> NON_STANDARD	<input checked="" type="checkbox"/> Normal <input checked="" type="checkbox"/> TBI <input type="checkbox"/> HDR <input type="checkbox"/> SRS
15e	100, 200, 300, 400, 500, 600, 700, 800, 900, 1000	<input checked="" type="checkbox"/> STANDARD <input type="checkbox"/> NON_STANDARD	<input checked="" type="checkbox"/> Normal <input checked="" type="checkbox"/> TBI <input type="checkbox"/> HDR <input type="checkbox"/> SRS
16e	100, 200, 300, 400, 500, 600, 700, 800, 900, 1000	<input checked="" type="checkbox"/> STANDARD <input type="checkbox"/> NON_STANDARD	<input checked="" type="checkbox"/> Normal <input checked="" type="checkbox"/> TBI <input type="checkbox"/> HDR <input type="checkbox"/> SRS
18e	100, 200, 300, 400, 500, 600, 700, 800, 900, 1000	<input checked="" type="checkbox"/> STANDARD <input type="checkbox"/> NON_STANDARD	<input checked="" type="checkbox"/> Normal <input checked="" type="checkbox"/> TBI <input type="checkbox"/> HDR <input type="checkbox"/> SRS
20e	100, 200, 300, 400, 500, 600, 700, 800, 900, 1000	<input checked="" type="checkbox"/> STANDARD <input type="checkbox"/> NON_STANDARD	<input checked="" type="checkbox"/> Normal <input checked="" type="checkbox"/> TBI <input type="checkbox"/> HDR <input type="checkbox"/> SRS
22e	100, 200, 300, 400, 500, 600, 700, 800, 900, 1000	<input checked="" type="checkbox"/> STANDARD <input type="checkbox"/> NON_STANDARD	<input checked="" type="checkbox"/> Normal <input checked="" type="checkbox"/> TBI <input type="checkbox"/> HDR <input type="checkbox"/> SRS

Table 5: Supported combinations for Primary Fluence Mode, Dose Rate, Energy, and High Dose Technique

3.1.5.2 4DITC

4DITC supports the following for Primary Fluence mode

Attribute Name	Tag	Type	Attribute Description
> Primary Fluence Mode Sequence	(3002,0050)	3	Sequence defining whether the primary fluence of the treatment beam uses a non-standard fluence-shaping. Only a single Item shall be permitted in this sequence.
>> Fluence Mode	(3002,0051)	1	Describes whether the fluence shaping is the standard mode for the beam or an alternate. Enumerated Values: STANDARD = Uses standard fluence-shaping NON_STANDARD = Uses a non-standard fluence-shaping mode
>> Fluence Mode ID	(3002,0052)	1C	Identifier for the specific fluence-shaping mode. Required if Fluence Mode (3002,0051) has value NON_STANDARD. 4DITC has supports the following mode IDs - SRS - FFF

Fluence modes IDs are displayed along with energy in 4DITC display

Fluence modes IDs are displayed along with energy in 4DITC display.

Example

6X- SRS, 6X- FFF and 10X-FFF

Nonstandard Fluence mode and ModeID SRS and FFF are supported for the following Energy and Dose Rate. But the following are machine specific – so it can be removed from DCS.

Nominal Beam Energy (MV/MeV) (300A,0114)	Dose Rate Set MU/Min (300A, 0115)	Primary Fluence Mode (3002,0051)*	Fluence Mode ID (3002,0052)
6X	800, 1000	NON_STANDARD	SRS
6X	140, 280, 420, ... 1400 [Steps of 140]	NON_STANDARD	FFF
10X	400, 800 ,... 2400 [Steps of 400]	NON_STANDARD	FFF

3.1.5.2.1 SOP Specific Conformance for the RT Beams Treatment Record storage SOP Class

Beam Limiting Device Position Sequence (300A,011A) only contains collimator jaws positions. It does not contain any MLC leaf position information. MLC leaf positions will not be reported within the RT Beams Treatment Record IOD.

Beams with Treatment Delivery Type (300A,00CE) set to OPEN_PORTFILM or TRMT_PORTFILM are Image Beams. Beams with Treatment Delivery Type set to TREATMENT are Treatment Beams.

All image beams attached to a treatment beam refer to the corresponding treatment beam. Similarly, all image beams attached to a setup beam refer to that setup beam. Beams refer to a Treatment Beam through the attribute Related Referenced Beam Number defined in section 4.2.1.

The Treatment Termination Status (3008,002A) specifies whether the treatment was completed or partially completed.

If MU Subtraction is set for an Image Beam, the treated MU count will be deducted from the related Treatment Beam. For Treatment Beams, MU Subtraction is always set. The following attributes are used to determine whether the MU Subtraction is set or not set:

Treatment Delivery Type (300A,00CE)	Related Beam Number (*)	Treatment Termination Status (3008, 002A)	MU Subtraction
OPEN_PORTFILM TRMT_PORTFILM	set	MACHINE	Set
OPEN_PORTFILM TRMT_PORTFILM	set	NORMAL	not set
TREATMENT	—	—	Set

Table 6: MU Subtraction Status



Note

The MU subtraction feature is available only on 4DITC console.

(*) Related Beam Number is a private tag added to the RT Beams Session Record module (see section 4.1.2).

RT Beams Treatment Record Extended Interface and Privatizations are described in section 4.

The following SOP specific conformance rules apply to 4DITC with implementation UID 'Varian Console Interface 4' or later.

Varian treatment delivery consoles support Treatment notes to be saved as part of RT Beams Treatment Record when patient session is closed. To store Treatment Notes in RT Beams Treatment Record, standard DICOM tag "Beam Description (300A, 00C3) is used.

Actual SSD is saved to RT Beams Treatment Record when patient session is closed. To store SSD in RT Beams Treatment Record, the Dicom tag "Source to Surface Distance (300A, 0130)" is used.

3.1.5.2.2 SOP specific conformance for the RT Image Storage SOP class

The 4DITC Entity only stores images with the Image Type (0008,0008) set to PORTAL.

3.1.5.3 Query/Retrieve SCU

3.1.5.3.1 Associated Real-World Activity

Varian treatment delivery consoles use the Query/Retrieve information model MOVE for retrieving patient data from the Management System. After a successful query, the Management System sends the requested data with the C-Store service.

Varian treatment delivery consoles uses the Query/Retrieve information model FIND for gathering information from the Management System. In order to determine whether a Beam was partially treated or completed, Varian treatment delivery consoles queries for several attributes in the RT Beams Treatment Record stored in the management.

3.1.5.3.2 Presentation Context Table

Presentation Context Table							
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation	TxA 2.5	4DITC 13.0
Name	UID	Name	UID				
Study Root Query/Retrieve Information Model - FIND	1.2.840.10008.5.1.4.1.2.2.1	DICOM Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None	Yes	Yes
Study Root Query/Retrieve Information Model - MOVE	1.2.840.10008.5.1.4.1.2.2.2	DICOM Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None	Yes	Yes

Table 7: Proposed Presentation Contexts for Query/Retrieve SCU

3.1.5.3.3 SOP Specific Conformance

The following Query/Retrieve SOP classes are used by Varian treatment delivery consoles as a Service Class User (SCU):

- C-Move RT Plan
- C-Move RT Treatment Summary Record
- C-Move RT Image
- C-Find RT Beams Treatment Record
- C-Find RT Plan
- C-Find RT Image (4DITC only)

3.1.5.3.3.1 SOP specific Conformance for the C-Move SOP Classes

For all C-Move SOP classes, the query key is always the SOP Instance UID of the particular DICOM IOD that 4DITC requests. There are no other matching criteria's for the C-Move key. All keys used for the C-Move service are defined in section B 1.1.

The C-Move service requires 4DITC to be an SCP of the C-Store service for the same DICOM IOD. For example whenever 4DITC is a SCU of C-Move RT Plan it implies that 4DITC is a SCP of C-Store RT Plan (see Table 1).

3.1.5.3.3.2 SOP specific Conformance for the C-Find RT Beams Treatment Record SOP Class

The C-Find RT Beams Treatment Record SOP class will be used for calculating the remaining MU. The remaining monitor units are calculated with the *Beam Meterset (300A,0086)* in the RT Fraction Scheme module (provided from the Plan IOD) minus the *Delivered Primary Meterset (3008, 0036)* (provided from the Beam Record Information) -see Table 18). If the monitor units were overridden, the Beam Record Information contains the overridden value in the *Specified Meterset (3008, 0042)*. In this case, the overridden *Specified Meterset (3008, 0042)* is used instead of the *Beam Meterset (300A,0086)* to calculate the remaining monitor units.

Calculation of Remaining MU when monitor units are not overridden:

Remaining MU = Beam Meterset (300A,0086) – Delivered Primary Meterset (3008,0036)

Calculation of Remaining MU when monitor units are overridden:

Remaining MU = Specified Meterset (3008, 0042) – Delivered Primary Meterset (3008,0036)

The Treatment Record key contains the matching criteria for the RT Beams Treatment Record. Whenever the key matches the particular RT Beams Treatment Record, the attributes defined in Table 18 (SCP column) gets filled in. Note that the Treatment Session Beam Sequence may contain one or more item. It is up to the Management System to decide whether for each Treatment Session Beam one Treatment Record key gets sent or if all Treatment Session Beams are sent within one Treatment Record key.

Only the last treated fraction is the fraction of interest.

3.1.5.3.3.3 SOP specific conformance for the C – Find RT Plan SOP class

Plans may be loaded into 4DITC without having them scheduled for the current session. Therefore 4DITC has to know how many treatment plans a patient has. This information gets retrieved with the C – Find RT Plan SOP Class. The Plan key contains the matching criteria and the placeholder for all attributes. The Plan key is defined in Table 17. The SOP Instance UID defined in the Plan key is the Plan Instance UID which will be used to load an unscheduled Plan in 4DITC.



Note

The unscheduled plan load feature is available only on 4DITC console.

3.1.5.3.3.4 SOP specific conformance for the C – Find RT Image SOP class

Since Portal Images are not referenced within the RT Plan, 4DITC queries the Portal Images from the Management System with the C – Find RT Image service SOP class. The Image key is defined in Table 16. The Referenced SOP Instance UID (i.e. the Plan Instance UID) and the Referenced Beam Number uniquely identifies the Beam, which 4DITC needs to query the Portal Images from. 4DITC uses the SOP Instance UID (i.e. the RT Image Instance UID) to retrieve previous acquired Portal Image. The C – Find confirmation returns as many Image keys as Portal Images stored in the Management System for that particular beam.

3.1.6 Association Acceptance Policy

The treatment delivery console entity accepts association requests for the supported service classes shown in **Figure 2**. Varian treatment delivery consoles accept only one Management System Application Entity for the possible association.

3.1.6.1 Storage SCP

3.1.6.1.1 Associated Real-World Activity

The patient data is sent from the Management System to Varian treatment delivery console using the C-Store service. This is the only service that Varian treatment delivery consoles support as an SCP.

3.1.6.1.2 Presentation Context Table

Presentation Context Table							
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation	TxA 2.5	4DITC 13.0
Name	UID	Name	UID				
RT Plan Storage	1.2.840.10008.5.1.4.1.1.481.5	DICOM Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None	Yes	Yes
		DICOM Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP	None	Yes	Yes
RT Image Storage	1.2.840.10008.5.1.4.1.1.481.1	DICOM Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None	No	Yes
		DICOM Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP	None	No	Yes
RT Treatment Summary Record Storage	1.2.840.10008.5.1.4.1.1.481.7	DICOM Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None	Yes	Yes
		DICOM Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP	None	Yes	Yes

Table 8: Acceptable Presentation Contexts for Storage SCP

3.1.6.1.3 SOP Specific Conformance for the Storage SOP class

Varian treatment delivery consoles are not an archive system. Thus DICOM IOD's are temporarily stored during a treatment session and deleted once the session is finished.

3.1.6.1.3.1 SOP specific conformance for RT Plan Storage SOP Class

3.1.6.1.3.2 SOP specific conformance for RT Image Storage SOP class (4DITC only)

The 4DITC Entity supports the following image types: DRR, PORTAL, and SIMULATOR.

To represent portal dose, RT Images of image type PORTAL are used. This is based on DICOM standard Part 3, section A.17.3 (RT Image IOD Module Table), Notes 2. The conversion between

portal image pixel values and portal dose is defined by the Modality LUT module through re-scale Slope and Intercept. The unit depends on the re-scale Type. The image type in Table 7 distinguishes the two types of portal doses:

Image Type	Meaning
DERIVED\SECONDARY\PORTAL\CALCULATED_DOSE	Portal dose predicted by a treatment planning system, i.e. an estimate of the dose that will be perceived by the portal imaging device.
ORIGINAL\PRIMARY\PORTAL\ACQUIRED_DOSE	Portal dose actually measured by the portal imaging device based on its calibration.

Table 9: Image Type

3.1.6.1.3.3 RT Image Geometrical Values

RT Images (used as reference images) require a sufficient amount of geometrical parameters that will define the position of RT Images with respect to the machine. The following parameters are required for proper operation of image verification applications associated with 4DITC:

- X-Ray Image Receptor Translation (3002,000D)
Value must be present.
- X-Ray Image Receptor Angle (3002,000E)
Value must be present.



No te *In the current release, only 0 is supported. Providing this value will ensure safe interpretation.*

- RT Image Position (3002,0012)
It is recommended to have this value defined. If the value is not defined, the application will assume that the image was centered on the X-Ray Image Receptor System.
- Radiation Machine SAD (3002,0022) or RT Image SID (3002,0026)
At least one of the two values must be present.
- Image Plane Pixel Spacing (3002,0011)
Value must be present.
- Gantry Angle (300A,011E)
Value must be present. This value shall represent the angle (in IEC GANTRY system coordinates) where the physical or virtual (in case of DRR) source of radiation is located.



No te *When kV images are used as Reference Images, this value describes the projection geometry. Therefore, this value may not coincide with the Gantry Hardware Readout of the linear accelerator since the kV Image radiation source may be on a different position than the linear accelerator' target focus.*

- RT Orientation (3002,0010)
In the future, it is recommended to have this value defined for images that have the RT Image Plane set to NORMAL (this value is required for NON-NORMAL images). This is because the DICOM standard does not unambiguously define the position of the RT Image pixel area in the IEC Image Receptor system when this value is missing. If this value is not provided, the application assumes that the value is (1,0,0,0,-1,0).

3.1.6.1.3.4 SOP specific conformance for the RT Treatment Summary Record SOP class

RT Treatment Summary Record IOD contains additional private tags defined in section 4.1.3.

3.1.6.2 Presentation Context Acceptance Criterion

The Varian treatment delivery console entity will accept the presentation contexts listed in Table 4: Proposed Presentation Contexts for Query/Retrieve SCU.

3.1.6.3 Transfer Syntax Selection Policies

Varian treatment delivery consoles accept both Implicit VR Little Endian and Explicit VR Little Endian as shown in Table 5. 4DITC does not prefer one presentation context over the other.

4. Communication profiles

4.1 Supported communications stacks

The Varian treatment delivery console entity provides DICOM V3.0 TCP/IP Network Communication Support as defined in PS 3.8 (part 8 of the DICOM V3.0 standard).

4.1.1 TCP/IP stack

The Varian treatment delivery console entity uses the TCP/IP stack of Microsoft Windows Operating Systems (Winsock).

4.1.1.1 Physical media support

The Varian treatment delivery console entity can run on any physical network media that is supported by the underlying hardware and operating system. These include, but are not limited to: thin, thick, and twisted-pair Ethernet, token ring network and FDDI.


5. Configuration

5.1 4DITC DICOM Configuration

4DITC is configured through the 4DITC Administration application.

5.1.1 AE Title/Presentation Address Mapping

4DITC Administration provides a mapping of an Application Entity Title to a Presentation Address. A Presentation Address consists of a host name and a port number. In 4DITC Administration, the related Application Entity Title, host name, and port number are grouped under the section Daemon (remote) that is within the DICOM Configuration box (see Figure 5).

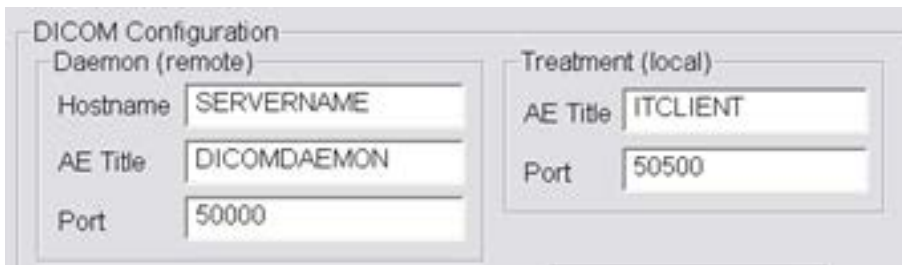

The screenshot shows a window titled "DICOM Configuration" with two main sections: "Daemon (remote)" and "Treatment (local)".

Section	Field	Value
Daemon (remote)	Hostname	SERVERNAME
	AE Title	DICOMDAEMON
	Port	50000
Treatment (local)	AE Title	ITCLIENT
	Port	50500

Figure 5: 4DITC Administration Setup

5.1.2 Configurable Parameters

The configurable parameters are located within the "DICOM Configuration" box of 4DITC Administration. The destination's AE Title, hostname or TCP/IP address, and port number can be configured under the "Daemon (remote)" section. The local AE Title and port number can be configured under the "Treatment (local)" section (see Figure 5).



No *In case warnings or errors are encountered after configuration, there are logs available to assist in determining the cause of the problem. 4DITC Administration has a "4D Console Application Configuration" section with a Log Level setting. When this Log Level is set to "Detailed" 4DITC writes more information to the log that will help in debugging the problem.*

5.2 TxA DICOM Configuration

The Treatment Preference Utility provides a mapping of an Application Entity Title to a Presentation Address. A Presentation Address consists of a host name and a port number. In Treatment Preferences Utility, the related Application Entity Title, host name, and port number are can be found in the Treatment Preference Utility, Advanced tab page (see Figure 6). The Client AE Title is the TXA application title, whereas Server AE Title represents the management system entity. Note that the connection can be tested only for TXA in the SCU and the management system in the SCP role within the Treatment Preference Utility Application.

DICOM Preferences

Client AETitle:

Client Port:

Client Mode:

Server Type:

Server AE Title:

Server Port:

Server IP Address: . . .

Figure 6: AE Title/Presentation Address Mapping

6. Media Interchange

The Varian treatment delivery console Application Entity does not support Media Interchange.

7. Support of Extended Character Sets

No dedicated support for Character Sets beyond the Default Repertoire is available. However, text fields containing characters not in the Default Character Repertoire when importing an instance will appear unchanged when re-exporting the same instance again

The following character set encodings are supported.

- Code Page 1252(Western Europe) or CP-1252
- Code Page 936 (Simplified Chinese)
- Code Page 932 (Japanese)

4DITC with implementation UID 'Varian Console Interface 6' or later supports:

- UTF-8

Correct display of characters not in the Default Character Repertoire depends on available/configured operating system support.

8. Security

8.1 Security Profiles

No Security Profiles are supported.

8.2 Association Level Security

The treatment delivery console checks the following values when determining whether to accept Association Open Requests:

- Called AE Title

8.3 Application Level Security

Local administrative rights are required for installing Varian treatment delivery consoles.

Appendix A Specialization

A.1 IOD Contents

A.1.1 Created SOP Instances

IODs created by TXA Entities are listed in Appendix C along with supported modules and its attributes.

A.1.2 Usage of Attributes from received IOD's

This section describes the required or optional presence of Type 1, 2 and 3 attributes which Varian treatment delivery consoles implement to pass the Plan IOD validation on load.

Type 1 attributes need to be present.

Type 2 attributes are distinguished as mandatory or optional attributes (similar to Type 1 and Type 3)

For all Type 2 RT Plan IOD attributes listed in Table 8, the roundtrip will be supported. This means that the attribute, if defined (attribute length greater than zero) while loading the RT Plan IOD, will be unchanged and present in the edited and saved RT Plan IOD.

For all Type 2 RT Plan IOD attributes not listed in Table 8 are deemed as optional and roundtrip is not supported.

Term used in the Handling column	Description
Mandatory	The attribute must be present and defined (attribute length greater than zero) if corresponding DICOM Module and Sequence is sent.
Optional	The attribute is being present with zero length or absent.

The table below summarizes the handling of RT Plan IOD Type 2 data elements in treatment delivery consoles.

Attribute Name	Tag	Module/Sequence	TxA v 2.5	4DITC v 13.0
Id	(0010, 0020)	Patient	Mandatory.	Mandatory.
Sex	(0010, 0040)	Patient	Optional.	Optional.
Name	(0010, 0010)	Patient	Mandatory.	Mandatory.
Birth Date	(0010, 0030)	Patient	Optional.	Optional.
Manufacturer	(0008, 0070)	General Equipment	Mandatory.	Mandatory
Leaf Position Boundaries	(300A, 00BE)	RT Beam Limiting Device	Mandatory.	Optional
Reviewer Name	(300E, 0008)	Approval	Mandatory.	Optional
Review Date	(300E, 0004)	Approval	Mandatory.	Optional
Treatment Date	(3008, 0250)	General Treatment Record	Mandatory.	Mandatory.

Treatment Time	(3008, 0251)	General Treatment Record	Mandatory.	Mandatory.
Treatment Machine Name	(300A, 00B2)	Beam	Mandatory.	Mandatory.
Radiation Type	(300A, 00C6)	Beam	Optional.	Optional.
Fraction Group Number	(300A, 0071)	Fraction Group	Mandatory.	Mandatory.
Operators Name	(0008, 1070)	RT General Plan	Optional.	Optional
Date	(300A, 0006)	RT General Plan	Mandatory.	Optional
Time	(300A, 0007)	RTGeneralPlan	Mandatory.	Optional
Cumulative Meterset Weight	(300A, 0134)	Control Point	Mandatory.	Mandatory
Table Top Vertical Position	(300A, 0128)	Control Point	Optional.	Optional
Table Top Longitudinal Position	(300A, 0129)	Control Point	Optional.	Optional
Table Top Lateral Position	(300A, 012A)	Control Point	Optional.	Optional
Isocenter Position	(300A, 012C)	Control Point	Optional.	Optional
Wedge Type	(300A, 00D3)	Wedge	Mandatory	Mandatory
Wedge Angle	(300A, 00D5)	Wedge	Mandatory	Mandatory
Wedge Factor	(300A, 00D6)	Wedge	Optional	Optional
Wedge Orientation	(300A, 00D8)	Wedge	Mandatory	Mandatory
Comp Material ID	(300A, 00E1)	Compensator	Mandatory	Mandatory
Source Comp Tray Distance	(300A, 00E6)	Compensator	Optional	Optional
Source Block Tray Distance	(300A, 00F6)	Block	Optional	Optional
Block Divergence	(300A, 00FA)	Block	Optional	Optional
Block Material ID	(300A, 00E1)	Block	Mandatory	Optional
Block Thickness	(300A, 0100)	Block	Optional	Optional
Block Transmission	(300A, 0102)	Block	Optional	Optional
Block Number Of Points	(300A, 0104)	Block	Mandatory	Optional
Block Data	(300A, 0106)	Block	Mandatory	Optional

Table 10: Treatment Delivery Console handling of RT Plan IOD DICOM Type 2 attributes

Type 3 attributes are optional and may be absent except the attributes listed in Table 9.

Attribute Name	Tag	Module/Sequence	TxA v2.5	4DITC v13.0
Beam Name	(300A,00C2)	Beam	Mandatory Unique beam identification for the User Interface.	Optional
Treatment Delivery Type	(300A,00CE)	Beam	Mandatory	Optional
Tolerance Table Label	(300A,0043)	Tolerance Table	Mandatory This attribute is being used for unique tolerance table identification.	Optional
Dose Reference Description	(300A,0016)	Dose Reference Sequence	Mandatory This attribute is being used for unique dose reference identification.	Mandatory

Table 11: Treatment Delivery Console handling of RT Plan IOD DICOM Type 3 attributes

A.2 Data Dictionary of Private Attributes

A.2.1 Privatization for RT Plan Storage SOP class

The DICOM Extended Interface is a private group added to the RT Plan IOD. This group contains an XML stream that contains the Plan Extended Interface described in **Appendix D**.

Attribute Name	Tag	Type	Attribute Description	VR
Extended Interface Data	(3253,xx00)	3	XML stream.	LT
Extended Interface Length	(3253,xx01)	3	Data length of the XML stream	IS
Extended Interface Format	(3253,xx02)	3	Extended Interface Format tag. A possible value is: 'ExtendedIF'	CS

Table 12: RT Plan Module Privatization

Attribute Name	Tag	Type	Attribute Description	VR
Fraction Group Sequence	(300A,0070)	1	-STANDARD DICOM- Introduces sequence of Fraction Groups in current Fraction Scheme.	SQ
> Referenced Beam Sequence	(300C,0080)	3	-STANDARD DICOM- Related instances of RT Dose (for grids, iso-dose curves and named/unnamed point doses).	SQ
>> Maximum Treatment Time	(3249,xx00)	3	The maximum treatment time, which should not be exceeded (in min). This item serves as a secondary safety limit besides the Beam Meterset (300A,0086) value itself.	DS

Table 13: RT Fraction Scheme Module Privatization

Attribute Name	Tag	Type	Attribute Description	VR
Beam Sequence	(300A,00B0)	1	-STANDARD DICOM- Introduces sequence of treatment beams for current RT Plan.	SQ
> Beam Secondary Name	(3243,xx09)	3	Second user-defined beam name	LO
> Accessory Sequence	(300A,0420)	3	-STANDARD DICOM- Introduces a Sequence of General Accessories associated with this Beam.	SH
>> General Accessory Type	(300A, 0423)	3	Additionally to the already defined terms, TRAY will be added defining accessory trays different than graticule, image detector and reticle. Defined Terms: GRATICULE IMAGE_DETECTOR RETICLE TRAY	SH

Table 14: RT Beams Module Privatization

A.2.2 Privatization for RT Beams Treatment Record Storage SOP class

Attribute Name	Tag	Type	Attribute Description	VR
Treatment Session Beam Sequence	(3008,0020)	1	-STANDARD DICOM- Introduces sequence of Beams administered during treatment session.	SQ
> Treatment Machine Note	(3251, xx00)	3	A description of the treatment machine details.	LO
>Beam Description	(300A,00C3)	3	User-defined description for delivered Beam. A treatment history note.	ST
> Treatment Session Beam Data	(3261,xx2A)	3	Extended interface in XML format.	OB
> Related Referenced Beam Number	(3243,xx28)	3	If TreatmentDeliveryType of the treated beam is either OPEN_PORTFILM or TRMT_PORTFILM then the Related Referenced Beam Number must be used instead of the Referenced Beam Number (300C, 0006). The Related Referenced Beam Number refers to the treatment field for which the image was taken.	IS
>Source to Surface Distance*	(300A,0130)	3	Source to Patient Surafce distance (mm)	DS

Table 15: RT Beams Session Record Module Privatization

A.2.3 Privatization for RT Treatment Summary Record Storage SOP class

*Note: Standard Extended attribute

Attribute Name	Tag	Type	Attribute Description	VR
Total Number of Fractions	(3265,xx00)	1	Total number of Fractions planned for the current plan and all its former plans.	SL
Last Treated Fraction	(3265,xx01)	1	The index of the last fraction treated across the current plan and all its former plans. In other words, this tag will always contain the fraction, which was last treated (completely or partially). So it will be the same as in the Fraction Status Summary Sequence (3008,0240) on the last item of the sequence in the tag Referenced Fraction Number (3008,0223), as soon as the sequence is not empty any more (so after the 1st treatment has got at least 1 MU). In case of completing a partial treatment, the plan's current fraction number is equal to <i>Last Treated Fraction (3265, 1001)</i> .	SL
Additional Dose Value Sequence	(3259,xx00)	3	Introduces sequence of Actual Session Dose Sequence. The sequence may contain one or more items. Sequence for additional Dose Information to a Reference Point. The ReferencePoint must be connected to Referenced Plan of this TreatmentSummary Record, but also the Dose of other Plans which have the same Reference Point have influence on this values.	SQ
> Actual Session Dose	(3259,xx02)	1C	Session Dose Delivered of Actual Session Required if Actual Session Dose Sequence is sent.	DS
> Daily Dose	(3259,xx04)	1C	Daily Dose of current day. Required if Actual Session Dose Sequence is sent.	DS
> Life Time Total Dose	(3259,xx06)	1C	Total Dose of Reference Point over all Plans. Required if Actual Session Dose Sequence is sent.	DS

Table 16: Treatment Summary Record Module Privatization

Appendix B DICOM Query Retrieve Service Class Object Matching Criteria (SCU Role)

This section describes the Conformance Statement for information query and data retrieval functions used in Treatment. They are implemented as the SCU role of the DICOM Query/Retrieve SOP Classes.

B.1 IOD Specific Matching Criteria

Table 15: Supported Query/Retrieve Levels for Query/Retrieve SCU shows the supported values for the tag Query/Retrieve Level (0008,0052):

Query/Retrieve Level		Value in (0008,0052)
Study Information		STUDY
Series Information		SERIES
Composite Object Instance Information	Plan Information	PLAN
	Treatment Record Information	TREATMENTRECORD
	Treatment Summary Record Information	TREATMENTSUMMARYRECORD
	Treatment Summary Record Information	TREATMENTSUMREC
Note: Treatment Delivery Console uses this value when association is established with Varian Console Interface 3 or higher.		

Table 17: Supported Query/Retrieve Levels for Query/Retrieve SCU



Note

In addition to the IMAGE value for the Composite Object Instance Level, we expect the following values for querying/retrieving the respective objects: PLAN, TREATMENTRECORD, TREATMENTSUMMARYRECORD, TREATMENTSUMREC.

B.1.1 Supported Keys

Varian treatment delivery consoles are not an SCP of any C-Find service. The tables in the following sub section show which keys the Treatment SCU is capable of generating query requests in order to perform a hierarchical search.

The following conventions are used to define the types of keys used by Treatment (SCU) in Query/Retrieve request sent to the management systems (SCP).

Symbol	Description
U	Unique Key Attribute
R	Required Key Attribute
O	Optional Key Attribute

B.1.1.1 Study Level

Description	Tag	Type
Query Level STUDY	(0008,0052)	R
Study Date	(0008,0020)	R
Study Time	(0008,0030)	R
Accession Number	(0008,0050)	R
Patient's Name	(0010,0010)	R
Patient ID	(0010,0020)	R
Study ID	(0020,0010)	R
Study Instance UID	(0020,000D)	U

Table 18: Study key

B.1.1.2 Series Level

Description	Tag	Type
Query Level SERIES	(0008,0052)	R
Modality	(0008,0060)	R
Series Number	(0020,0011)	R
Series Instance UID	(0020,000E)	U
Study Instance UID	(0020,000D)	U

Table 19: Series key

B.1.1.3 Composite Object Instance Level

B.1.1.3.1 Plan

Description	Tag	Type
Query Level PLAN	(0008,0052)	R
SOP Instance UID	(0008,0018)	U
Series Instance UID	(0020,000E)	U
Study Instance UID	(0020,000D)	U
Patient's Name	(0010,0010)	O
Patient ID	(0010,0020)	O
Plan Label	(300A,0002)	O
Plan Date	(300A,0006)	O
Plan Time	(300A,0007)	O
Number of Beams	(300A,0080)	O
Referenced RT Plan Sequence	(300C,0002)	O
>Referenced SOP Class UID	(0008,1150)	O
>Referenced SOP Instance UID	(0008,1155)	O
>RT Plan Relationship	(300A,0055)	O
Field Type	(3257,xx00)	O
Plan Type	(3257,xx01)	O

Table 20: Plan key

B.1.1.3.2 Treatment Record Key

Description	Tag	Type
Query Level TREATMENTRECORD	(0008,0052)	R
SOP Instance UID	(0008,0018)	U
Series Instance UID	(0020,000E)	U
Study Instance UID	(0020,000D)	U
Referenced SOP Class UID	(0008,1150)	O
Referenced SOP Instance UID	(0008,1155)	O
Treatment Date	(3008,0250)	O
Treatment Time	(3008,0251)	O
Referenced Fraction Group Number	(300C,0022)	O
Treatment Session Beam Sequence	(3008,0020)	O
>Referenced Beam Number	(300C,0006)	O
>Treatment Delivery Type	(300A,00CE)	O
>Treatment Termination Status	(3008,002A)	O
>Delivered Primary Meterset	(3008,0036)	O

>Current Fraction Number	(3008,0022)	O
>Referenced Calculated Dose Reference Sequence	(3008,0090)	O
>>Referenced Dose Reference Number	(300C,0051)	O
>>Calculated Dose Reference Value	(3008,0076)	O
>Control Point Delivery Sequence	(3008,0040)	O
>>Referenced Control Point Index	(300C,00F0)	O
>>Specified Meterset	(3008,0042)	O
>>Override Sequence	(3008,0060)	O
>>>Override Parameter Pointer	(3008,0062)	O

Table 21: Treatment Record key

B.1.1.3.3 Treatment Summary Record

Description	Tag	Type
Query Level - VMS Console System 6.5: TREATMENTSUMMARYRECORD - VMS Console System 8.8 and VMS Console System 8.8 QA: TREATMENTSUMMARYREC	(0008,0052)	R
Referenced SOP Class UID	(0008,1150)	O
Referenced SOP Instance UID	(0008,1155)	O
Current Treatment Status	(3008,0200)	O
Number of Fractions Delivered	(3008,005A)	O
Treatment Summary Calculated Dose Reference Sequence	(3008,0050)	O
>Referenced Dose Reference Number	(300C,0051)	O
>Dose Reference Description	(300A,0016)	O
>Cumulative Dose to Dose Reference	(3008,0052)	O

Table 22: Treatment Record key

Appendix C IOD Details

C.1 Supported IODs

The following tables define the modules that are and are not supported for a particular IOD. For specific IOD details, refer to Related Documents [2].

The “Not supported” entries in the Support column indicate that the import of module is not supported or it is discarded on import of this IOD and will never appear in exported IOD.

RT Plan IOD Module Table

IE	Module	Reference	DICOM Usage	Support
Patient	Patient	C.7.1.1	M	
Study	General Study	C.7.2.1	M	
	Patient Study	C.7.2.2	U	Not supported
Series	RT Series	C.8.8.1	M	
Frame of Reference	Frame Of Reference	C.7.4.1	U	
Equipment	General Equipment	C.7.5.1	M	
Plan	RT General Plan	C.8.8.9	M	
	RT Prescription	C.8.8.10	U	
	RT Tolerance Tables	C.8.8.11	U	
	RT Patient Setup	C.8.8.12	U	
	RT Fraction Scheme	C.8.8.13	U	
	RT Beams	C.8.8.14	C	
	RT Brachy Application Setups	C.8.8.15	C	Not supported
	Approval	C.8.8.16	U	
	Audio	C.10.3	U	Not supported
	SOP Common	C.12.1	M	
	DICOM Extended Interface	Private module (see C.2.13)	C	Additional features are supported with this module.

Table 23: RT Plan IOD Module

RT Beams Treatment Record IOD Module Table

IE	Module	Reference	DICOM Usage	Notes
Patient	Patient	C.7.1.1	M	
Study	General Study	C.7.2.1	M	
	Patient Study	C.7.2.2	U	Not supported
Series	RT Series	C.8.8.1	M	
Equipment	General Equipment	C.7.5.1	M	
Treatment Record	RT General Treatment Record	C.8.8.17	M	
	RT Patient Setup	C.8.8.12	U	Not supported
	RT Treatment Machine Record	C.8.8.18	M	
	Measured Dose Reference Record	C.8.8.19	U	Not supported
	Calculated Dose Reference Record	C.8.8.20	U	Not supported
	RT Beams Session Record	C.8.8.21	M	
	RT Treatment Summary Record	C.8.8.22	U	Not supported
	Curve	C.10.2	U	Not supported
	SOP Common	C.12.1	M	

Table 24: RT Beams Treatment Record IOD Module

RT Treatment Summary Record Module Table

IE	Module	Reference	DICOM Usage	Notes
Patient	Patient	C.7.1.1	M	
Study	General Study	C.7.2.1	M	
	Patient Study	C.7.2.2	U	Not supported
Series	RT Series	C.8.8.1	M	
Equipment	General Equipment	C.7.5.1	M	
Treatment Record	RT General Treatment Record	C.8.8.17	M	
	RT Treatment Summary	C.8.8.23	M	

	Record			
	Curve	C.10.2	U	Not supported
	SOP Common	C.12.1	M	

Table 25: RT Treatment Summary Record Module

RT Image IOD Module Table (4DITC only)

IE	Module	Reference	DICOM Usage	Notes
Patient	Patient	C.7.1.1	M	—
Study	General Study	C.7.2.1	M	—
	Patient Study	C.7.2.2	U	Not supported
Series	RT Series	C.8.8.1	M	—
Frame Of Reference	Frame of Reference	C.7.4.1	U	—
Equipment	General Equipment	C.7.5.1	M	—
Image	General Image	C.7.6.1	M	—
	Image Pixel	C.7.6.1	M	—
	Contrast/bolus	C.7.6.3	C	Not supported
	Cine	C.7.6.5	C	Not supported
	Multi-Frame	C.7.6.6	C	Not supported
	RT Image	C.8.8.2	M	—
	Modality LUT	C.11.1	U	—
	VOI LUT	C.11.2	U	—
	Approval	C.8.8.16	U	—
	Curve	C.10.2	U	—
	Audio	C.10.3	U	Not supported
	SOP Common	C.12.1	M	—

Table 26: RT Image Module (4DITC only)

C.2 Modules and Attributes

For better reference with DICOM Standard, section titles of the following sub-sections are decorated with section number of DICOM Standard Part 3 where the corresponding Module Attribute table can be found. The first four columns in the following tables contain definitions from the DICOM standard. All references in those columns refer to the DICOM standard and not to this document.

Note that Varian treatment delivery consoles only support roundtrip with RT Plan IOD's. Thus this section is focusing solely on RT Plan IOD attributes.

Column TxA v2.5 and 4DITC v13.0 support describes for each attribute whether it is supported thus maintained when loading the plan for these respective consoles.

Value in "TXA Model Support" column	Description
*** not supported ***	Attribute is unknown and therefore ignored by TXA. This means that the Roundtrip (load, edit and save) will result in erasing this attribute in the RT Plan IOD..
Roundtrip supported.	Complete roundtrip is guaranteed. Loading, editing and saving will maintain (unless edited) the original value in the exported RT Plan IOD.

C.2.1 Patient – C.7.1.1

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
Patient's Name	(0010,0010)	2	Patient's full name.	Roundtrip supported.	Roundtrip supported.
Patient ID	(0010,0020)	2	Primary hospital identification number or code for the patient.	Roundtrip supported.	Roundtrip supported.
Issuer of Patient ID	(0010,0021)	3	Identifier of the Assigning Authority that issued the Patient ID.	*** not supported ***	Not supported
Patient's Birth Date	(0010,0030)	2	Birth date of the patient.	Roundtrip supported.	Roundtrip supported.
Patient's Sex	(0010,0040)	2	Sex of the named patient. Enumerated Values: M = male F = female O = other	Roundtrip supported.	Roundtrip supported.
Referenced Patient Sequence	(0008,1120)	3	A sequence that provides reference to a Patient SOP Class/Instance pair. Only a single Item shall be permitted in this Sequence.	*** not supported ***	Not supported
> Referenced SOP Class UID	(0008,1150)	1C	Uniquely identifies the referenced SOP Class. Required if Referenced Patient Sequence (0008,1120) is sent.	*** not supported ***	Not supported

IOD Details, Supported Keys

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
> Referenced SOP Instance UID	(0008,1155)	1C	Uniquely identifies the referenced SOP Instance. Required if Referenced Patient Sequence (0008,1120) is sent.	*** not supported ***	Not supported
Patient's Birth Time	(0010,0032)	3	Birth time of the Patient.	Roundtrip supported.	Roundtrip supported.
Other Patient IDs	(0010,1000)	3	Other identification numbers or codes used to identify the patient.	Roundtrip supported.	Roundtrip supported.
Other Patient Names	(0010,1001)	3	Other names used to identify the patient.	*** not supported ***	Not supported
Ethnic Group	(0010,2160)	3	Ethnic group or race of the patient.	Roundtrip supported.	Roundtrip supported.
Patient Comments	(0010,4000)	3	User-defined additional information about the patient.	Roundtrip supported.d.	Roundtrip supported.
Patient Identify Removed	(0012,0062)	3	The true identity of the patient has been removed from the Attributes and the Pixel Data Enumerated Values: YES NO	*** not supported ***	Not supported
De-identification Method	(0012,0063)	1C	A description or label of the mechanism or method use to remove the patient's identity. May be multi-valued if successive de-identification steps have been performed. Note: This may be used to describe the extent or thoroughness of the de- identification, for example whether or not the de-identification is for a "Limited Data Set" (as per HIPAA Privacy Rule). Required if Patient Identity Removed (0012,0062) is present and has a value of YES and De-identification Method Code Sequence (0012,0064) is not present.	*** not supported ***	Not supported

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
De-identification Method Code Sequence	(0012,0064)	1C	A code describing the mechanism or method use to remove the patient's identity. One or more Items shall be present. Multiple items are used if successive de-identification steps have been performed Required if Patient Identity Removed (0012,0062) is present and has a value of YES and De-identification Method (0012,0063) is not present.	*** not supported ***	Not supported
> Code Value	(0008,0100)	1C	See Section 8.1. Required if a sequence item is present.	*** not supported ***	Not supported
> Coding Scheme Designator	(0008,0102)	1C	See Section 8.2. Required if a sequence item is present.	*** not supported ***	Not supported
> Coding Scheme Version	(0008,0103)	1C	See Section 8.2. Required if a sequence item is present and the value of Coding Scheme Designator (0008,0102) is not sufficient to identify the Code Value (0008,0100) unambiguously.	*** not supported ***	Not supported
> Code Meaning	(0008,0104)	1C	See Section 8.3. Required if a sequence item is present.	*** not supported ***	Not supported

C.2.2 General Study - C.7.2.1

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
Study Instance UID	(0020,000D)	1	Unique identifier for the Study.	Roundtrip supported	Roundtrip supported
Study Date	(0008,0020)	2	Date the Study started.	Roundtrip supported	Roundtrip supported
Study Time	(0008,0030)	2	Time the Study started.	Roundtrip supported	Roundtrip supported
Referring Physician's Name	(0008,0090)	2	Name of the patient's referring physician	Roundtrip supported	Roundtrip supported
Referring Physician Identification Sequence	(0008,0096)	3	Identification of the patient's referring physician. Only a single item shall be permitted in this sequence.	*** not supported ***	Not supported

IOD Details, General Study - C.7.2.1

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
> Person Identification Code Sequence	(0040,1101)	1	A coded entry which identifies a person. The Code Meaning attribute, though it will be encoded with a VR of LO, may be encoded according to the rules of the PN VR (e.g. caret '^' delimiters shall separate name components), except that a single component (i.e. the whole name unseparated by caret delimiters) is not permitted. Name component groups for use with multi-byte character sets are permitted, as long as they fit within the 64 characters (the length of the LO VR). One or more Items may be permitted in this Sequence.	*** not supported ***	Not supported
>> Code Value	(0008,0100)	1C	See Section 8.1. Required if a sequence item is present.	*** not supported ***	Not supported
>> Coding Scheme Designator	(0008,0102)	1C	See Section 8.2. Required if a sequence item is present.	*** not supported ***	Not supported
>> Coding Scheme Version	(0008,0103)	1C	See Section 8.2. Required if a sequence item is present and the value of Coding Scheme Designator (0008,0102) is not sufficient to identify the Code Value (0008,0100) unambiguously.	*** not supported ***	Not supported
>> Code Meaning	(0008,0104)	1C	See Section 8.3. Required if a sequence item is present.	*** not supported ***	Not supported
> Person's Address	(0040,1102)	3	Person's mailing address	*** not supported ***	Not supported
> Person's Telephone Numbers	(0040,1103)	3	Person's telephone number(s)	*** not supported ***	Not supported
> Institution Name	(0008,0080)	1C	Institution or organization to which the identified individual is responsible or accountable. Shall not be present if Institution Code Sequence (0008,0082) is present.	*** not supported ***	Not supported
> Institution Address	(0008,0081)	3	Mailing address of the institution or organization to which the identified individual is responsible or accountable.	*** not supported ***	Not supported

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
> Institution Code Sequence	(0008,0082)	1C	Institution or organization to which the identified individual is responsible or accountable. Shall not be present if Institution Name (0008,0080) is present. Only a single Item shall be permitted in this Sequence.	*** not supported ***	Not supported
>> Code Value	(0008,0100)	1C	See Section 8.1. Required if a sequence item is present.	*** not supported ***	Not supported
>> Coding Scheme Designator	(0008,0102)	1C	See Section 8.2. Required if a sequence item is present.	*** not supported ***	Not supported
>> Coding Scheme Version	(0008,0103)	1C	See Section 8.2. Required if a sequence item is present and the value of Coding Scheme Designator (0008,0102) is not sufficient to identify the Code Value (0008,0100) unambiguously.	*** not supported ***	Not supported
>> Code Meaning	(0008,0104)	1C	See Section 8.3. Required if a sequence item is present.	*** not supported ***	Not supported
Study ID	(0020,0010)	2	User or equipment generated Study identifier.	Roundtrip supported	Roundtrip supported
Accession Number	(0008,0050)	2	A RIS generated number that identifies the order for the Study.	Roundtrip supported	Roundtrip supported
Study Description	(0008,1030)	3	Institution-generated description or classification of the Study (component) performed.	Roundtrip supported	Roundtrip supported
Physician(s) of Record	(0008,1048)	3	Names of the physician(s) who are responsible for overall patient care at time of Study (see Section C.7.3.1 for Performing Physician)	Roundtrip supported	Roundtrip supported
Physician(s) of Record Identification Sequence	(0008,1049)	3	Identification of the physician(s) who are responsible for overall patient care at time of Study. One or more items shall be included in this sequence. If more than one Item, the number and order shall correspond to the value of Physician(s) of Record (0008,1048), if present.	*** not supported ***	Not supported

IOD Details, General Study - C.7.2.1

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
> Person Identification Code Sequence	(0040,1101)	1	A coded entry which identifies a person. The Code Meaning attribute, though it will be encoded with a VR of LO, may be encoded according to the rules of the PN VR (e.g. caret '^' delimiters shall separate name components), except that a single component (i.e. the whole name unseparated by caret delimiters) is not permitted. Name component groups for use with multi-byte character sets are permitted, as long as they fit within the 64 characters (the length of the LO VR). One or more Items may be permitted in this Sequence.	*** not supported ***	Not supported
>> Code Value	(0008,0100)	1C	See Section 8.1. Required if a sequence item is present.	*** not supported ***	Not supported
>> Coding Scheme Designator	(0008,0102)	1C	See Section 8.2. Required if a sequence item is present.	*** not supported ***	Not supported
>> Coding Scheme Version	(0008,0103)	1C	See Section 8.2. Required if a sequence item is present and the value of Coding Scheme Designator (0008,0102) is not sufficient to identify the Code Value (0008,0100) unambiguously.	*** not supported ***	Not supported
>> Code Meaning	(0008,0104)	1C	See Section 8.3. Required if a sequence item is present.	*** not supported ***	Not supported
> Person's Address	(0040,1102)	3	Person's mailing address	*** not supported ***	Not supported
> Person's Telephone Numbers	(0040,1103)	3	Person's telephone number(s)	*** not supported ***	Not supported
> Institution Name	(0008,0080)	1C	Institution or organization to which the identified individual is responsible or accountable. Shall not be present if Institution Code Sequence (0008,0082) is present.	*** not supported ***	Not supported
> Institution Address	(0008,0081)	3	Mailing address of the institution or organization to which the identified individual is responsible or accountable.	*** not supported ***	Not supported

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
> Institution Code Sequence	(0008,0082)	1C	Institution or organization to which the identified individual is responsible or accountable. Shall not be present if Institution Name (0008,0080) is present. Only a single Item shall be permitted in this Sequence.	*** not supported ***	Not supported
>> Code Value	(0008,0100)	1C	See Section 8.1. Required if a sequence item is present.	*** not supported ***	Not supported
>> Coding Scheme Designator	(0008,0102)	1C	See Section 8.2. Required if a sequence item is present.	*** not supported ***	Not supported
>> Coding Scheme Version	(0008,0103)	1C	See Section 8.2. Required if a sequence item is present and the value of Coding Scheme Designator (0008,0102) is not sufficient to identify the Code Value (0008,0100) unambiguously.	*** not supported ***	Not supported
>> Code Meaning	(0008,0104)	1C	See Section 8.3. Required if a sequence item is present.	*** not supported ***	Not supported
Name of Physician(s) Reading Study	(0008,1060)	3	Names of the physician(s) reading the Study.	*** not supported ***	Not supported
Physician(s) Reading Study Identification Sequence	(0008,1062)	3	Identification of the physician(s) reading the Study. One or more items shall be included in this sequence. If more than one Item, the number and order shall correspond to the value of Name of Physician(s) Reading Study (0008,1060), if present.	*** not supported ***	Not supported
> Person Identification Code Sequence	(0040,1101)	1	A coded entry which identifies a person. The Code Meaning attribute, though it will be encoded with a VR of LO, may be encoded according to the rules of the PN VR (e.g. caret '^' delimiters shall separate name components), except that a single component (i.e. the whole name unseparated by caret delimiters) is not permitted. Name component groups for use with multi-byte character sets are permitted, as long as they fit within the 64 characters (the length of the LO VR). One or more Items may be permitted in this Sequence.	*** not supported ***	Not supported

IOD Details, General Study - C.7.2.1

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
>> Code Value	(0008,0100)	1C	See Section 8.1. Required if a sequence item is present.	*** not supported ***	Not supported
>> Coding Scheme Designator	(0008,0102)	1C	See Section 8.2. Required if a sequence item is present.	*** not supported ***	Not supported
>> Coding Scheme Version	(0008,0103)	1C	See Section 8.2. Required if a sequence item is present and the value of Coding Scheme Designator (0008,0102) is not sufficient to identify the Code Value (0008,0100) unambiguously.	*** not supported ***	Not supported
>> Code Meaning	(0008,0104)	1C	See Section 8.3. Required if a sequence item is present.	*** not supported ***	Not supported
> Person's Address	(0040,1102)	3	Person's mailing address	*** not supported ***	Not supported
> Person's Telephone Numbers	(0040,1103)	3	Person's telephone number(s)	*** not supported ***	Not supported
> Institution Name	(0008,0080)	1C	Institution or organization to which the identified individual is responsible or accountable. Shall not be present if Institution Code Sequence (0008,0082) is present.	*** not supported ***	Not supported
> Institution Address	(0008,0081)	3	Mailing address of the institution or organization to which the identified individual is responsible or accountable.	*** not supported ***	Not supported
> Institution Code Sequence	(0008,0082)	1C	Institution or organization to which the identified individual is responsible or accountable. Shall not be present if Institution Name (0008,0080) is present. Only a single Item shall be permitted in this Sequence.	*** not supported ***	Not supported
>> Code Value	(0008,0100)	1C	See Section 8.1. Required if a sequence item is present.	*** not supported ***	Not supported
>> Coding Scheme Designator	(0008,0102)	1C	See Section 8.2. Required if a sequence item is present.	*** not supported ***	Not supported

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
>> Coding Scheme Version	(0008,0103)	1C	See Section 8.2. Required if a sequence item is present and the value of Coding Scheme Designator (0008,0102) is not sufficient to identify the Code Value (0008,0100) unambiguously.	*** not supported ***	Not supported
>> Code Meaning	(0008,0104)	1C	See Section 8.3. Required if a sequence item is present.	*** not supported ***	Not supported
Referenced Study Sequence	(0008,1110)	3	A sequence that provides reference to a Study SOP Class/Instance pair. The sequence may have zero or more Items.	*** not supported ***	Not supported
> Referenced SOP Class UID	(0008,1150)	1C	Uniquely identifies the referenced SOP Class. Required if Referenced Study Sequence (0008,1110) is sent.	*** not supported ***	Not supported
> Referenced SOP Instance UID	(0008,1155)	1C	Uniquely identifies the referenced SOP Instance. Required if Referenced Study Sequence (0008,1110) is sent.	*** not supported ***	Not supported
Procedure Code Sequence	(0008,1032)	3	A Sequence that conveys the type of procedure performed. One or more Items may be included in this Sequence.	*** not supported ***	Not supported
> Code Value	(0008,0100)	1C	See Section 8.1. Required if a sequence item is present.	*** not supported ***	Not supported
> Coding Scheme Designator	(0008,0102)	1C	See Section 8.2. Required if a sequence item is present.	*** not supported ***	Not supported
> Coding Scheme Version	(0008,0103)	1C	See Section 8.2. Required if a sequence item is present and the value of Coding Scheme Designator (0008,0102) is not sufficient to identify the Code Value (0008,0100) unambiguously.	*** not supported ***	Not supported
> Code Meaning	(0008,0104)	1C	See Section 8.3. Required if a sequence item is present.	*** not supported ***	Not supported

C.2.3 Frame of Reference – C.7.4.1

Attribute Name	Tag	Type	Attribute Description	TXA V2.5	4DITC v13.0
Frame of Reference UID	(0020,0052)	1	Uniquely identifies the frame of reference for a Series.	Roundtrip supported	Not supported

IOD Details, General Equipment – C.7.5.1

Attribute Name	Tag	Type	Attribute Description	TXA V2.5	4DITC v13.0
Position Reference Indicator	(0020,1040)	2	Part of the imaging target used as a reference	Roundtrip supported	Not supported

C.2.4 General Equipment – C.7.5.1

Attribute Name	Tag	Type	Attribute Description	TXA V2.5	4DITC v13.0
Manufacturer	(0008,0070)	2	Manufacturer of the equipment that produced the composite instances.	Roundtrip supported	Roundtrip supported
Institution Name	(0008,0080)	3	Institution where the equipment that produced the composite instances is located.	Roundtrip supported	Roundtrip supported
Institution Address	(0008,0081)	3	Mailing address of the institution where the equipment that produced the composite instances is located.	Roundtrip supported	Roundtrip supported
Station Name	(0008,1010)	3	User defined name identifying the machine that produced the composite instances.	Roundtrip supported	Roundtrip supported
Institutional Department Name	(0008,1040)	3	Department in the institution where the equipment that produced the composite instances is located.	Roundtrip supported	Roundtrip supported
Manufacturer's Model Name	(0008,1090)	3	Manufacturer's model name of the equipment that produced the composite instances.	Roundtrip supported	Roundtrip supported
Device Serial Number	(0018,1000)	3	Manufacturer's serial number of the equipment that produced the composite instances.	Roundtrip supported	Roundtrip supported
Software Version(s)	(0018,1020)	3	Manufacturer's designation of software version of the equipment that produced the composite instances.	Roundtrip supported	Roundtrip supported
Spatial Resolution	(0018,1050)	3	The inherent limiting resolution in mm of the acquisition equipment for high contrast objects for the data gathering and reconstruction technique chosen. If variable across the images of the series, the value at the image center.	Roundtrip supported	Roundtrip supported

Attribute Name	Tag	Type	Attribute Description	TXA V2.5	4DITC v13.0
Date of Last Calibration	(0018,1200)	3	Date when the image acquisition device calibration was last changed in any way. Multiple entries may be used for additional calibrations at other times. See C.7.5.1.1.1 for further explanation.	Roundtrip supported	Roundtrip supported
Time of Last Calibration	(0018,1201)	3	Time when the image acquisition device calibration was last changed in any way. Multiple entries may be used. See C.7.5.1.1.1 for further explanation.	Roundtrip supported	Roundtrip supported
Pixel Padding Value	(0028,0120)	3	Value of pixels not present in the native image added to an image to pad to rectangular format. See C.7.5.1.1.2 for further explanation. Note: The Value Representation of this Attribute is determined by the value of Pixel Representation (0028,0103).	Roundtrip supported	Roundtrip supported

C.2.5 RT Series – C.8.8.1

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
Modality	(0008,0060)	1	Type of equipment that originally acquired the data. Enumerated Values: RTIMAGE = RT Image RTDOSE = RT Dose RTSTRUCT = RT Structure Set RTPLAN = RT Plan RTRECORD = RT Treatment Record See C.8.8.1.1.	Roundtrip supported	Roundtrip supported
Series Instance UID	(0020,000E)	1	Unique identifier of the series.	Roundtrip supported	Roundtrip supported
Series Number	(0020,0011)	2	A number that identifies this series.	Roundtrip supported	Roundtrip supported
Series Description	(0008,103E)	3	User provided description of the series.	Roundtrip supported.	Roundtrip supported.

IOD Details, RT Series – C.8.8.1

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
Referenced Performed Procedure Step Sequence	(0008,1111)	3	Uniquely identifies the Performed Procedure Step SOP Instance to which the Series is related (e.g. a Modality or General-Purpose Performed Procedure Step SOP Instance). One or more items may be included in this sequence.	*** not supported ***	Not supported
> Referenced SOP Class UID	(0008,1150)	1C	Uniquely identifies the referenced SOP Class. Required if Referenced Performed Procedure Step Sequence (0008,1111) is sent.	*** not supported ***	Not supported
> Referenced SOP Instance UID	(0008,1155)	1C	Uniquely identifies the referenced SOP Instance. Required if Referenced Performed Procedure Step Sequence (0008,1111) is sent.	*** not supported ***	Not supported
Request Attributes Sequence	(0040,0275)	3	Sequence that contains attributes from the Imaging Service Request. The sequence may have one or more Items.	*** not supported ***	Not supported
> Requested Procedure ID	(0040,1001)	1	Identifier that identifies the Requested Procedure in the Imaging Service Request.	*** not supported ***	Not supported
> Reason for the Requested Procedure	(0040,1002)	3	Reason for requesting this procedure.	*** not supported ***	Not supported
> Reason for Requested Procedure Code Sequence	(0040,100A)	3	Coded Reason for requesting this procedure.	*** not supported ***	Not supported
>> Code Value	(0008,0100)	1C	See Section 8.1. Required if a sequence item is present.	*** not supported ***	Not supported
>> Coding Scheme Designator	(0008,0102)	1C	See Section 8.2. Required if a sequence item is present.	*** not supported ***	Not supported
>> Coding Scheme Version	(0008,0103)	1C	See Section 8.2. Required if a sequence item is present and the value of Coding Scheme Designator (0008,0102) is not sufficient to identify the Code Value (0008,0100) unambiguously.	*** not supported ***	Not supported
>> Code Meaning	(0008,0104)	1C	See Section 8.3. Required if a sequence item is present.	*** not supported ***	Not supported
> Scheduled Procedure Step ID	(0040,0009)	1	Identifier that identifies the Scheduled Procedure Step.	*** not supported ***	Not supported

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
> Scheduled Procedure Step Description	(0040,0007)	3	Institution-generated description or classification of the Scheduled Procedure Step to be performed.	*** not supported ***	Not supported
> Scheduled Protocol Code Sequence	(0040,0008)	3	Sequence describing the Scheduled Protocol following a specific coding scheme. This sequence contains one or more Items.	*** not supported ***	Not supported
>> Code Value	(0008,0100)	1C	See Section 8.1. Required if a sequence item is present.	*** not supported ***	Not supported
>> Coding Scheme Designator	(0008,0102)	1C	See Section 8.2. Required if a sequence item is present.	*** not supported ***	Not supported
>> Coding Scheme Version	(0008,0103)	1C	See Section 8.2. Required if a sequence item is present and the value of Coding Scheme Designator (0008,0102) is not sufficient to identify the Code Value (0008,0100) unambiguously.	*** not supported ***	Not supported
>> Code Meaning	(0008,0104)	1C	See Section 8.3. Required if a sequence item is present.	*** not supported ***	Not supported
>> Protocol Context Sequence	(0040,0440)	3	Sequence that specifies the context for the Scheduled Protocol Code Sequence Item. One or more items may be included in this sequence.	*** not supported ***	Not supported
>>> Code Value	(0008,0100)	1C	See Section 8.1. Required if a sequence item is present.	*** not supported ***	Not supported
>>> Coding Scheme Designator	(0008,0102)	1C	See Section 8.2. Required if a sequence item is present.	*** not supported ***	Not supported
>>> Coding Scheme Version	(0008,0103)	1C	See Section 8.2. Required if a sequence item is present and the value of Coding Scheme Designator (0008,0102) is not sufficient to identify the Code Value (0008,0100) unambiguously.	*** not supported ***	Not supported
>>> Code Meaning	(0008,0104)	1C	See Section 8.3. Required if a sequence item is present.	*** not supported ***	Not supported
>>> Content Item Modifier Sequence	(0040,0441)	3	Sequence that specifies modifiers for a Protocol Context Content Item. One or more items may be included in this sequence. See Section C.4.10.1.	*** not supported ***	Not supported
>>>> Code Value	(0008,0100)	1C	See Section 8.1. Required if a sequence item is present.	*** not supported ***	Not supported

IOD Details, RT Series – C.8.8.1

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
>>>> Coding Scheme Designator	(0008,0102)	1C	See Section 8.2. Required if a sequence item is present.	*** not supported ***	Not supported
>>>> Coding Scheme Version	(0008,0103)	1C	See Section 8.2. Required if a sequence item is present and the value of Coding Scheme Designator (0008,0102) is not sufficient to identify the Code Value (0008,0100) unambiguously.	*** not supported ***	Not supported
>>>> Code Meaning	(0008,0104)	1C	See Section 8.3. Required if a sequence item is present.	*** not supported ***	Not supported
Performed Procedure Step ID	(0040,0253)	3	User or equipment generated identifier of that part of a Procedure that has been carried out within this step.	*** not supported ***	Not supported
Performed Procedure Step Start Date	(0040,0244)	3	Date on which the Performed Procedure Step started.	*** not supported ***	Not supported
Performed Procedure Step Start Time	(0040,0245)	3	Time on which the Performed Procedure Step started.	*** not supported ***	Not supported
Performed Procedure Step Description	(0040,0254)	3	Institution-generated description or classification of the Procedure Step that was performed.	*** not supported ***	Not supported
Performed Protocol Code Sequence	(0040,0260)	3	Sequence describing the Protocol performed for this Procedure Step. One or more Items may be included in this Sequence.	*** not supported ***	Not supported
> Code Value	(0008,0100)	1C	See Section 8.1. Required if a sequence item is present.	*** not supported ***	Not supported
> Coding Scheme Designator	(0008,0102)	1C	See Section 8.2. Required if a sequence item is present.	*** not supported ***	Not supported
> Coding Scheme Version	(0008,0103)	1C	See Section 8.2. Required if a sequence item is present and the value of Coding Scheme Designator (0008,0102) is not sufficient to identify the Code Value (0008,0100) unambiguously.	*** not supported ***	Not supported
> Code Meaning	(0008,0104)	1C	See Section 8.3. Required if a sequence item is present.	*** not supported ***	Not supported

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
> Protocol Context Sequence	(0040,0440)	3	Sequence that specifies the context for the Performed Protocol Code Sequence Item. One or more items may be included in this sequence.	*** not supported ***	Not supported
>> Value Type	(0040,A040)	1	The type of the value encoded in this name-value Item. Defined Terms: DATETIME DATE TIME PNAME UIDREF TEXT CODE NUMERIC.	*** not supported ***	Not supported
>> Concept Name Code Sequence	(0040,A043)	1	Coded concept name of this name-value Item.	*** not supported ***	Not supported
>>> Code Value	(0008,0100)	1C	See Section 8.1. Required if a sequence item is present.	*** not supported ***	Not supported
>>> Coding Scheme Designator	(0008,0102)	1C	See Section 8.2. Required if a sequence item is present.	*** not supported ***	Not supported
>>> Coding Scheme Version	(0008,0103)	1C	See Section 8.2. Required if a sequence item is present and the value of Coding Scheme Designator (0008,0102) is not sufficient to identify the Code Value (0008,0100) unambiguously.	*** not supported ***	Not supported
>>> Code Meaning	(0008,0104)	1C	See Section 8.3. Required if a sequence item is present.	*** not supported ***	Not supported
>> DateTime	(0040,A120)	1C	Datetime value for this name-value Item. Required if Value Type (0040,A040) is DATETIME.	*** not supported ***	Not supported
>> Date	(0040,A121)	1C	Date value for this name-value Item. Required if Value Type (0040,A040) is DATE.	*** not supported ***	Not supported
>> Time	(0040,A122)	1C	Time value for this name-value Item. Required if Value Type (0040,A040) is TIME.	*** not supported ***	Not supported
>> Person Name	(0040,A123)	1C	Person name value for this name-value Item. Required if Value Type (0040,A040) is PNAME.	*** not supported ***	Not supported

IOD Details, RT Series – C.8.8.1

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
>> UID	(0040,A124)	1C	UID value for this name-value Item. Required if Value Type (0040,A040) is UIDREF.	*** not supported ***	Not supported
>> Text Value	(0040,A160)	1C	Text value for this name-value Item. Required if Value Type (0040,A040) is TEXT.	*** not supported ***	Not supported
>> Concept Code Sequence	(0040,A168)	1C	Coded concept value of this name-value Item. Required if Value Type (0040,A040) is CODE.	*** not supported ***	Not supported
>>> Code Value	(0008,0100)	1C	See Section 8.1. Required if a sequence item is present.	*** not supported ***	Not supported
>>> Coding Scheme Designator	(0008,0102)	1C	See Section 8.2. Required if a sequence item is present.	*** not supported ***	Not supported
>>> Coding Scheme Version	(0008,0103)	1C	See Section 8.2. Required if a sequence item is present and the value of Coding Scheme Designator (0008,0102) is not sufficient to identify the Code Value (0008,0100) unambiguously.	*** not supported ***	Not supported
>>> Code Meaning	(0008,0104)	1C	See Section 8.3. Required if a sequence item is present.	*** not supported ***	Not supported
>> Numeric Value	(0040,A30A)	1C	Numeric value for this name-value Item. Required if Value Type (0040,A040) is NUMERIC.	*** not supported ***	Not supported
>> Measurement Units Code Sequence	(0040,08EA)	1C	Units of measurement for a numeric value in this namevalue Item. Required if Value Type (0040,A040) is NUMERIC.	*** not supported ***	Not supported
>>> Code Value	(0008,0100)	1C	See Section 8.1. Required if a sequence item is present.	*** not supported ***	Not supported
>>> Coding Scheme Designator	(0008,0102)	1C	See Section 8.2. Required if a sequence item is present.	*** not supported ***	Not supported
>>> Coding Scheme Version	(0008,0103)	1C	See Section 8.2. Required if a sequence item is present and the value of Coding Scheme Designator (0008,0102) is not sufficient to identify the Code Value (0008,0100) unambiguously.	*** not supported ***	Not supported
>>> Code Meaning	(0008,0104)	1C	See Section 8.3. Required if a sequence item is present.	*** not supported ***	Not supported

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
>> Content Item Modifier Sequence	(0040,0441)	3	Sequence that specifies modifiers for a Protocol Context Content Item. One or more items may be included in this sequence. See Section C.4.10.1.	*** not supported ***	Not supported
>>> Value Type	(0040,A040)	1	The type of the value encoded in this name-value Item. Defined Terms: DATETIME DATE TIME PNAME UIDREF TEXT CODE NUMERIC.	*** not supported ***	Not supported
>>> Concept Name Code Sequence	(0040,A043)	1	Coded concept name of this name-value Item.	*** not supported ***	Not supported
>>>> Code Value	(0008,0100)	1C	See Section 8.1. Required if a sequence item is present.	*** not supported ***	Not supported
>>>> Coding Scheme Designator	(0008,0102)	1C	See Section 8.2. Required if a sequence item is present.	*** not supported ***	Not supported
>>>> Coding Scheme Version	(0008,0103)	1C	See Section 8.2. Required if a sequence item is present and the value of Coding Scheme Designator (0008,0102) is not sufficient to identify the Code Value (0008,0100) unambiguously.	*** not supported ***	Not supported
>>>> Code Meaning	(0008,0104)	1C	See Section 8.3. Required if a sequence item is present.	*** not supported ***	Not supported
>>> DateTime	(0040,A120)	1C	Datetime value for this name-value Item. Required if Value Type (0040,A040) is DATETIME.	*** not supported ***	Not supported
>>> Date	(0040,A121)	1C	Date value for this name-value Item. Required if Value Type (0040,A040) is DATE.	*** not supported ***	Not supported
>>> Time	(0040,A122)	1C	Time value for this name-value Item. Required if Value Type (0040,A040) is TIME.	*** not supported ***	Not supported
>>> Person Name	(0040,A123)	1C	Person name value for this name-value Item. Required if Value Type (0040,A040) is PNAME.	*** not supported ***	Not supported

IOD Details, RT Series – C.8.8.1

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
>>> UID	(0040,A124)	1C	UID value for this name-value Item. Required if Value Type (0040,A040) is UIDREF.	*** not supported ***	Not supported
>>> Text Value	(0040,A160)	1C	Text value for this name-value Item. Required if Value Type (0040,A040) is TEXT.	*** not supported ***	Not supported
>>> Concept Code Sequence	(0040,A168)	1C	Coded concept value of this name-value Item. Required if Value Type (0040,A040) is CODE.	*** not supported ***	Not supported
>>>> Code Value	(0008,0100)	1C	See Section 8.1. Required if a sequence item is present.	*** not supported ***	Not supported
>>>> Coding Scheme Designator	(0008,0102)	1C	See Section 8.2. Required if a sequence item is present.	*** not supported ***	Not supported
>>>> Coding Scheme Version	(0008,0103)	1C	See Section 8.2. Required if a sequence item is present and the value of Coding Scheme Designator (0008,0102) is not sufficient to identify the Code Value (0008,0100) unambiguously.	*** not supported ***	Not supported
>>>> Code Meaning	(0008,0104)	1C	See Section 8.3. Required if a sequence item is present.	*** not supported ***	Not supported
>>> Numeric Value	(0040,A30A)	1C	Numeric value for this name-value Item. Required if Value Type (0040,A040) is NUMERIC.	*** not supported ***	Not supported
>>> Measurement Units Code Sequence	(0040,08EA)	1C	Units of measurement for a numeric value in this namevalue Item. Required if Value Type (0040,A040) is NUMERIC.	*** not supported ***	Not supported
>>>> Code Value	(0008,0100)	1C	See Section 8.1. Required if a sequence item is present.	*** not supported ***	Not supported
>>>> Coding Scheme Designator	(0008,0102)	1C	See Section 8.2. Required if a sequence item is present.	*** not supported ***	Not supported
>>>> Coding Scheme Version	(0008,0103)	1C	See Section 8.2. Required if a sequence item is present and the value of Coding Scheme Designator (0008,0102) is not sufficient to identify the Code Value (0008,0100) unambiguously.	*** not supported ***	Not supported
>>>> Code Meaning	(0008,0104)	1C	See Section 8.3. Required if a sequence item is present.	*** not supported ***	Not supported

C.2.6 RT General Plan – C.8.8.9

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
RT Plan Label	(300A,0002)	1	User-defined label for treatment plan.	Roundtrip supported	Roundtrip supported
RT Plan Name	(300A,0003)	3	User-defined name for treatment plan.	Roundtrip supported	Roundtrip supported
RT Plan Description	(300A,0004)	3	User-defined description of treatment plan.	Roundtrip supported	Roundtrip supported
Instance Number	(0020,0013)	3	A number that identifies this object instance.	*** not supported ***	Not supported
Operators' Name	(0008,1070)	2	Name of operator(s) creating treatment plan.	Roundtrip supported	Roundtrip supported
RT Plan Date	(300A,0006)	2	Date treatment plan was last modified.	Roundtrip supported	Roundtrip supported
RT Plan Time	(300A,0007)	2	Time treatment plan was last modified.	Roundtrip supported	Roundtrip supported
Treatment Protocols	(300A,0009)	3	Planned treatment protocols.	*** not supported ***	Not supported
Plan Intent	(300A,000A)	3	Intent of this plan. Defined Terms: CURATIVE = curative therapy on patient PALLIATIVE = palliative therapy on patient PROPHYLACTIC = preventative therapy on patient VERIFICATION = verification of patient plan using phantom MACHINE_QA = Quality assurance of the delivery machine (independently of a specific patient) RESEARCH = Research project SERVICE = Machine repair or maintenance operation	Roundtrip supported	Roundtrip supported
Treatment Sites	(300A,000B)	3	Planned treatment sites.	*** not supported ***	Not supported
RT Plan Geometry	(300A,000C)	1	Describes whether RT Plan is based on patient or treatment device geometry. See C.8.8.9.1. Defined Terms: PATIENT = RT Structure Set exists TREATMENT_DEVICE = RT Structure Set does not exist	Roundtrip supported	Roundtrip supported

IOD Details, RT General Plan – C.8.8.9

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
Referenced Structure Set Sequence	(300C,0060)	1C	Introduces sequence of one Class/Instance pair describing instance of RT Structure Set on which the RT Plan is based. Only a single item shall be permitted in this sequence. Required if RT Plan Geometry (300A,000C) is PATIENT.	Roundtrip supported	Roundtrip supported
> Referenced SOP Class UID	(0008,1150)	1C	Uniquely identifies the referenced SOP Class. Required if Referenced Structure Set Sequence (300C,0060) is sent.	Roundtrip supported	Roundtrip supported
> Referenced SOP Instance UID	(0008,1155)	1C	Uniquely identifies the referenced SOP Instance. Required if Referenced Structure Set Sequence (300C,0060) is sent.	Roundtrip supported	Roundtrip supported
Referenced Dose Sequence	(300C,0080)	3	Introduces sequence of related SOP Class/Instance pairs describing related instances of RT Dose (for grids and named/unnamed point doses). One or more items may be included in this sequence. See Note 1.	*** not supported ***	Not supported
> Referenced SOP Class UID	(0008,1150)	1C	Uniquely identifies the referenced SOP Class. Required if Referenced RT Dose Sequence (300C,0080) is sent.	*** not supported ***	Not supported
> Referenced SOP Instance UID	(0008,1155)	1C	Uniquely identifies the referenced SOP Instance. Required if Referenced RT Dose Sequence (300C,0080) is sent.	*** not supported ***	Not supported
Referenced RT Plan Sequence	(300C,0002)	3	Introduces sequence of related SOP Class/Instance pairs describing related instances of RT Plan. One or more items may be included in this sequence.	Roundtrip supported	Roundtrip supported
> Referenced SOP Class UID	(0008,1150)	1C	Uniquely identifies the referenced SOP Class. Required if Referenced RT Plan Sequence (300C,0002) is sent.	Roundtrip supported	Roundtrip supported
> Referenced SOP Instance UID	(0008,1155)	1C	Uniquely identifies the referenced SOP Instance. Required if Referenced RT Plan Sequence (300C,0002) is sent.	Roundtrip supported	Roundtrip supported

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
> RT Plan Relationship	(300A,0055)	1C	Relationship of referenced plan with respect to current plan. Required if Referenced RT Plan Sequence (300C,0002) is sent. Defined Terms: PRIOR = plan delivered prior to current treatment ALTERNATIVE = alternative plan prepared for current treatment PREDECESSOR = plan used in derivation of current plan VERIFIED_PLAN = plan which is verified using the current plan. This value shall only be used if Plan Intent (300A,000A) is present and has a value of VERIFICATION.	Roundtrip supported	Roundtrip supported
Beam Line Data Table Version	(300B,1008)	3	Version Number that is set for Look-up Table (and/or for each beam tune in Look-up Table in future)	*** not supported ***	Not supported
Plan Integrity Sequence	(3287,XX00)	3	Introduces sequence of checksum on dose-relevant data in this RT Plan. Exactly one item may be included in this sequence.	Roundtrip supported	Roundtrip supported
> Plan Integrity Hash	(3287,XX01)	1	Hash value calculated from selected data of this RT Plan along a specific algorithm whose version number is specified in Plan Integrity Hash Version (3287,xx02).	Roundtrip supported	Roundtrip supported
> Plan Integrity Hash Version	(3287,XX02)	1	Version of hash algorithm used to calculate value of Plan Integrity Hash (3287,xx01).	Roundtrip supported	Roundtrip supported

C.2.7 RT Prescription – C.8.8.10

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
Prescription Description	(300A,000E)	3	User-defined description of treatment prescription.	Roundtrip supported	Roundtrip supported
Dose Reference Sequence	(300A,0010)	3	Introduces sequence of Dose References. One or more items may be included in this sequence.	Roundtrip supported	Roundtrip supported

IOD Details, RT Prescription – C.8.8.10

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
> Dose Reference Number	(300A,0012)	1C	Identification number of the Dose Reference. The value of Dose Reference Number (300A,0012) shall be unique within the RT Plan in which it is created. Required if Dose Reference Sequence (300A,0012) is sent.	Roundtrip supported	Roundtrip supported
> Dose Reference UID	(300A,0013)	3	A unique identifier for a Dose Reference that can be used to link the same entity across multiple RT Plan objects.	*** not supported ***	Roundtrip supported
> Dose Reference Structure Type	(300A,0014)	1C	Structure type of Dose Reference. Required if Dose Reference Sequence (300A,0010) is sent. Defined Terms: POINT = dose reference point specified as ROI VOLUME = dose reference volume specified as ROI COORDINATES = point specified by Dose Reference Point Coordinates (300A,0018) SITE = dose reference clinical site	Roundtrip supported	Roundtrip supported
> Dose Reference Description	(300A,0016)	3	User-defined description of Dose Reference.	Roundtrip supported	Roundtrip supported
> Referenced ROI Number	(3006,0084)	1C	Uniquely identifies ROI representing the dose reference specified by ROI Number (3006,0022) in Structure Set ROI Sequence (3006,0020) in Structure Set Module within RT Structure Set in Referenced Structure Set Sequence (300C,0060) in RT General Plan Module. Required if Dose Reference Structure Type (300A,0014) is POINT or VOLUME and Dose Reference Sequence (300A,0010) is sent.	Roundtrip supported	Roundtrip supported

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
> Dose Reference Point Coordinates	(300A,0018)	1C	Coordinates (x,y,z) of Reference Point in the patient based coordinate system described in C.7.6.2.1.1 (mm). Required if Dose Reference Structure Type (300A,0014) is COORDINATES and Dose Reference Sequence (300A,0010) is sent.	Roundtrip supported	Roundtrip supported
> Nominal Prior Dose	(300A,001A)	3	Dose (in Gy) from prior treatment to this Dose Reference (e.g. from a previous course of treatment).	Roundtrip supported	Roundtrip supported
> Dose Reference Type	(300A,0020)	1C	Type of Dose Reference. Required if Dose Reference Sequence (300A,0010) is sent. Defined Terms: TARGET = treatment target (corresponding to GTV, PTV, or CTV in ICRU50) ORGAN_AT_RISK = Organ at Risk (as defined in ICRU50)	Roundtrip supported	Roundtrip supported
> Constraint Weight	(300A,0021)	3	Relative importance of satisfying constraint, where high values represent more important constraints.	Roundtrip supported	Roundtrip supported
> Delivery Warning Dose	(300A,0022)	3	The dose (in Gy) which when reached or exceeded should cause some action to be taken.	Roundtrip supported	Roundtrip supported
> Delivery Maximum Dose	(300A,0023)	3	The maximum dose (in Gy) which can be delivered to the dose reference.	Roundtrip supported	Roundtrip supported
> Target Minimum Dose	(300A,0025)	3	Minimum permitted dose (in Gy) to Dose Reference if Dose Reference Type (300A,0020) is TARGET.	*** not supported ***	Roundtrip supported
> Target Prescription Dose	(300A,0026)	3	Prescribed dose (in Gy) to Dose Reference if Dose Reference Type (300A,0020) is TARGET.	Roundtrip supported	Roundtrip supported
> Target Maximum Dose	(300A,0027)	3	Maximum permitted dose (in Gy) to Dose Reference if Dose Reference Type (300A,0020) is TARGET.	Roundtrip supported	Roundtrip supported
> Referenced Patient Volume Id	(3267,XX00)	3		*** not supported **	Not supported

IOD Details, RT Tolerance Tables – C.8.8.11

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
> Target Underdose Volume Fraction	(300A,0028)	3	Maximum permitted fraction (in percent) of Target to receive less than the Target Prescription Dose if Dose Reference Type (300A,0020) is TARGET and Dose Reference Structure Type (300A,0014) is VOLUME. See C.8.8.10.1.	*** not supported ***	Not supported
> Organ at Risk Full-volume Dose	(300A,002A)	3	Maximum dose (in Gy) to entire Dose Reference if Dose Reference Type (300A,0020) is ORGAN_AT_RISK and Dose Reference Structure Type (300A,0014) is VOLUME.	*** not supported ***	Not supported
> Organ at Risk Limit Dose	(300A,002B)	3	Maximum permitted dose (in Gy) to any part of Dose Reference if Dose Reference Type (300A,0020) is ORGAN_AT_RISK and Dose Reference Structure Type (300A,0014) is VOLUME.	Roundtrip supported	Roundtrip supported
> Organ at Risk Maximum Dose	(300A,002C)	3	Maximum dose (in Gy) to non-overdosed part of Dose Reference if Dose Reference Type (300A,0020) is ORGAN_AT_RISK and Dose Reference Structure Type (300A,0014) is VOLUME.	Roundtrip supported	Roundtrip supported
> Organ at Risk Overdose Volume Fraction	(300A,002D)	3	Maximum permitted fraction (in percent) of the Organ at Risk to receive more than the Organ at Risk Maximum Dose if Dose Reference Type (300A,0020) is ORGAN_AT_RISK and Dose Reference Structure Type (300A,0014) is VOLUME.	Roundtrip supported	Roundtrip supported

C.2.8 RT Tolerance Tables – C.8.8.11

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
Tolerance Table Sequence	(300A,0040)	3	Introduces sequence of tolerance tables to be used for delivery of treatment plan. One or more items may be included in this sequence. See Note 1.	Roundtrip supported	Roundtrip supported

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
> Tolerance Table Number	(300A,0042)	1C	Identification number of the Tolerance Table. The value of Tolerance Table Number (300A,0042) shall be unique within the RT Plan in which it is created. Required if Tolerance Table Sequence (300A,0040) is sent.	Roundtrip supported.	Roundtrip supported.
> Tolerance Table Label	(300A,0043)	3	User-defined label for Tolerance Table.	Roundtrip supported	Roundtrip supported.
> Gantry Angle Tolerance	(300A,0044)	3	Maximum permitted difference (in degrees) between planned and delivered Gantry Angle.	Roundtrip supported	Roundtrip supported.
> Gantry Pitch Angle Tolerance	(300A,014E)	3	Maximum permitted difference (in degrees) between planned and delivered Gantry Pitch Angle.	*** not supported ***	*** not supported ***
> Beam Limiting Device Angle Tolerance	(300A,0046)	3	Maximum permitted difference (in degrees) between planned and delivered Beam Limiting Device Angle.	Roundtrip supported	Roundtrip supported
> Beam Limiting Device Tolerance Sequence	(300A,0048)	3	Introduces sequence of beam limiting device (collimator) tolerances. One or more items may be included in this sequence.	Roundtrip supported	Roundtrip supported
>> RT Beam Limiting Device Type	(300A,00B8)	1C	Type of beam limiting device (collimator). Required if Beam Limiting Device Tolerance Sequence (300A,0048) is sent. Enumerated Values: X = symmetric jaw pair in IEC X direction Y = symmetric jaw pair in IEC Y direction ASYMX = asymmetric jaw pair in IEC X direction ASYMY = asymmetric pair in IEC Y direction MLCX = multileaf (multi-element) jaw pair in IEC X direction MLCY = multileaf (multi-element) jaw pair in IEC Y direction	Roundtrip supported	Roundtrip supported

IOD Details, RT Tolerance Tables – C.8.8.11

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
>> Beam Limiting Device Position Tolerance	(300A,004A)	1C	Maximum permitted difference (in mm) between planned and delivered leaf (element) or jaw positions for current beam limiting device (collimator). Required if Beam Limiting Device Tolerance Sequence (300A,0048) is sent.	Roundtrip supported	Roundtrip supported
> Patient Support Angle Tolerance	(300A,004C)	3	Maximum permitted difference (in degrees) between planned and delivered Patient Support Angle.	Roundtrip supported	Roundtrip supported
> Table Top Eccentric Angle Tolerance	(300A,004E)	3	Maximum permitted difference (in degrees) between planned and delivered Table Top Eccentric Angle.	Roundtrip supported	Roundtrip supported
> Table Top Pitch Angle Tolerance	(300A,004F)	3	Maximum permitted difference (in degrees) between the planned and delivered Table Top Pitch Angle.	Beam will be valid if the tag is not available or has any value. This value will be read and ignored.	*** not supported ***
> Table Top Roll Angle Tolerance	(300A,0050)	3	Maximum permitted difference (in degrees) between the planned and delivered Table Top Roll Angle.	Beam will be valid if the tag is not available or has any value. This value will be read and ignored.	*** not supported ***
> Table Top Vertical Position Tolerance	(300A,0051)	3	Maximum permitted difference (in mm) between planned and delivered Table Top Vertical Position.	Roundtrip supported	Roundtrip supported
> Table Top Longitudinal Position Tolerance	(300A,0052)	3	Maximum permitted difference (in mm) between planned and delivered Table Top Longitudinal Position.	Roundtrip supported	Roundtrip supported
> Table Top Lateral Position Tolerance	(300A,0053)	3	Maximum permitted difference (in mm) between planned and delivered Table Top Lateral Position.	Roundtrip supported	Roundtrip supported

C.2.9 RT Patient Setup – C.8.8.12

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
Patient Setup Sequence	(300A,0180)	1	Introduces sequence of patient setup data for current plan. One or more items may be included in this sequence.	Roundtrip supported	Roundtrip supported
> Patient Setup Number	(300A,0182)	1	Identification number of the Patient Setup. The value of Patient Setup Number (300A,0182) shall be unique within the RT Plan in which it is created.	Roundtrip supported	Roundtrip supported
> Patient Setup Label	(300A,0183)	3	The user-defined label for the patient setup.	*** not supported ***	*** not supported ***
> Patient Position	(0018,5100)	1C	Patient position descriptor relative to the equipment. Required if Patient Additional Position (300A,0184) is not present. See Section C.7.3.1.1.2 for Defined Terms and further explanation.	Roundtrip supported	Roundtrip supported
> Patient Additional Position	(300A,0184)	1C	User-defined additional description of patient position. Required if Patient Position (0018,5100) is not present.	*** not supported ***	*** not supported ***
> Referenced Image Setup Sequence	(300A,0401)	3	Introduces sequence of setup verification images for this patient setup. One or more items may be included in this sequence. See C.8.8.12.1.1	Roundtrip supported	*** not supported ***
>> Setup Image Comment	(300A,0402)	3	Comment on the Setup Image.	*** not supported ***	*** not supported ***
>> Referenced SOP Class UID	(0008,1150)	1	Uniquely identifies the referenced SOP Class.	*** not supported ***	*** not supported ***
>> Referenced SOP Instance UID	(0008,1155)	1	Uniquely identifies the referenced SOP Instance.	*** not supported ***	*** not supported ***

IOD Details, RT Patient Setup – C.8.8.12

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
>> Referenced Frame Number	(0008,1160)	1	Identifies the frame numbers within the Referenced SOP Instance to which the reference applies. The first frame shall be denoted as frame number 1. Note: This Attribute may be multi-valued. Required if the Referenced SOP Instance is a multi-frame image and the reference does not apply to all frames.	*** not supported ***	*** not supported ***
> Fixation Device Sequence	(300A,0190)	3	Introduces sequence of Fixation Devices used in Patient Setup. One or more items may be included in this sequence.	*** not supported ***	*** not supported ***
>> Fixation Device Type	(300A,0192)	1C	Type of Fixation Device used during in Patient Setup. Required if Fixation Device Sequence (300A,0190) is sent. Defined Terms: BITEBLOCK HEADFRAME MASK MOLD CAST HEADREST BREAST_BOARD BODY_FRAME VACUUM_MOLD WHOLE_BODY_POD RECTAL_BALLOON	*** not supported ***	*** not supported ***
>> Fixation Device Label	(300A,0194)	2C	User-defined label identifier for Fixation Device. Required if Fixation Device Sequence (300A,0190) is sent.	*** not supported ***	*** not supported ***
>> Fixation Device Description	(300A,0196)	3	User-defined description of Fixation Device.	*** not supported ***	*** not supported ***
>> Fixation Device Position	(300A,0198)	3	Position/Notch number of Fixation Device.	*** not supported ***	*** not supported ***

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
>> Fixation Device Pitch Angle	(300A,0199)	3	The Fixation Device Pitch Angle, i.e. orientation of PITCHED FIXATION DEVICE coordinate system with respect to IEC PATIENT SUPPORT coordinate system (degrees). Pitching is the rotation around IEC PATIENT SUPPORT X-axis.	*** not supported ***	*** not supported ***
>> Fixation Device Roll Angle	(300A,019A)	3	The Fixation Device Roll Angle, i.e. orientation of ROLLED FIXATION DEVICE coordinate system with respect to IEC PITCHED FIXATION DEVICE coordinate system (degrees). Rolling is the rotation around IEC PATIENT SUPPORT Y-axis.	*** not supported ***	*** not supported ***
>> Accessory Code	(300A,00F9)	3	An identifier for the accessory intended to be read by a device such as a bar-code reader.	*** not supported ***	*** not supported ***
> Shielding Device Sequence	(300A,01A0)	3	Introduces sequence of Shielding Devices used in Patient Setup. One or more items may be included in this sequence.	*** not supported ***	*** not supported ***
>> Shielding Device Type	(300A,01A2)	1C	Type of Shielding Device used in Patient Setup. Required if Shielding Device Sequence (300A,01A0) is sent. Defined Terms: GUM EYE GONAD	*** not supported ***	*** not supported ***
>> Shielding Device Label	(300A,01A4)	2C	User-defined label for Shielding Device. Required if Shielding Device Sequence (300A,01A0) is sent.	*** not supported ***	*** not supported ***
>> Shielding Device Description	(300A,01A6)	3	User-defined description of Shielding Device.	*** not supported ***	*** not supported ***
>> Shielding Device Position	(300A,01A8)	3	Position/Notch number of Shielding Device.	*** not supported ***	*** not supported ***
>> Accessory Code	(300A,00F9)	3	An identifier for the accessory intended to be read by a device such as a bar-code reader.	*** not supported ***	*** not supported ***

IOD Details, RT Patient Setup – C.8.8.12

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
> Setup Technique	(300A,01B0)	3	Setup Technique used in Patient Setup. Defined Terms: ISOCENTRIC FIXED_SSD TBI BREAST_BRIDGE SKIN_APPOSITION	*** not supported ***	Roundtrip supported
> Setup Technique Description	(300A,01B2)	3	User-defined description of Setup Technique.	Roundtrip supported	Roundtrip supported
> Setup Device Sequence	(300A,01B4)	3	Introduces sequence of devices used for patient alignment in Patient Setup. One or more items may be included in this sequence.	*** not supported ***	*** not supported ***
>> Setup Device Type	(300A,01B6)	1C	Type of Setup Device used for Patient alignment. Required if Setup Device Sequence (300A,01B4) is sent. Defined Terms: LASER_POINTER DISTANCE_METER TABLE_HEIGHT MECHANICAL_PTR ARC	*** not supported ***	*** not supported ***
>> Setup Device Label	(300A,01B8)	2C	User-defined label for Setup Device used for patient alignment. Required if Setup Device Sequence (300A,01B4) is sent.	*** not supported ***	*** not supported ***
>> Setup Device Description	(300A,01BA)	3	User-defined description for Setup Device used for patient alignment.	*** not supported ***	*** not supported ***
>> Setup Device Parameter	(300A,01BC)	2C	Setup Parameter for Setup Device in appropriate IEC 61217 coordinate system. Units shall be mm for distances and degrees for angles. Required if Setup Device Sequence (300A,01B4) is sent.	*** not supported ***	*** not supported ***
>> Setup Reference Description	(300A,01D0)	3	User-defined description of Setup Reference used for patient alignment.	*** not supported ***	*** not supported ***

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
> Table Top Vertical Setup Displacement	(300A,01D2)	3	Vertical Displacement in IEC TABLE TOP coordinate system (in mm) relative to initial Setup Position, i.e. vertical offset between patient positioning performed using setup and treatment position.	*** not supported ***	Roundtrip supported
> Table Top Longitudinal Setup Displacement	(300A,01D4)	3	Longitudinal Displacement in IEC TABLE TOP coordinate system (in mm) relative to initial Setup Position, i.e. longitudinal offset between patient positioning performed using setup and treatment position.	*** not supported ***	Roundtrip supported
> Table Top Lateral Setup Displacement	(300A,01D6)	3	Lateral Displacement in IEC TABLE TOP coordinate system (in mm) relative to initial Setup Position, i.e. lateral offset between patient positioning performed using setup and treatment position.	*** not supported ***	Roundtrip supported

C.2.10 RT Fraction Scheme – C.8.8.13

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
Fraction Group Sequence	(300A,0070)	1	Introduces sequence of Fraction Groups in current Fraction Scheme. One or more items may be included in this sequence.	Roundtrip supported	Roundtrip supported
> Fraction Group Number	(300A,0071)	1	Identification number of the Fraction Group. The value of Fraction Group Number (300A,0071) shall be unique within the RT Plan in which it is created.	Roundtrip supported	Roundtrip supported
> Fraction Group Description	(300A,0072)	3	The user defined description for the fraction group.	*** not supported ***	*** not supported ***
> Referenced Dose Sequence	(300C,0080)	3	Introduces sequence of related SOP Class/Instance pairs describing related instances of RT Dose (for grids, isodose curves and named/unnamed point doses). One or more items may be included in this sequence. See Note 1.	*** not supported ***	*** not supported ***

IOD Details, RT Fraction Scheme – C.8.8.13

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
>> Referenced SOP Class UID	(0008,1150)	1C	Uniquely identifies the referenced SOP Class. Required if Referenced Dose Sequence (300C,0080) is sent.	*** not supported ***	*** not supported ***
>> Referenced SOP Instance UID	(0008,1155)	1C	Uniquely identifies the referenced SOP Instance. Required if Referenced Dose Sequence (300C,0080) is sent.	*** not supported ***	*** not supported ***
> Referenced Dose Reference Sequence	(300C,0050)	3	Introduces sequence of Dose References for the current Fraction Group. One or more items may be included in this sequence.	*** not supported ***	*** not supported ***
>> Referenced Dose Reference Number	(300C,0051)	1C	Uniquely identifies Dose Reference specified by Dose Reference Number (300A,0012) within Dose Reference Sequence (300A,0010) in RT Prescription Module. Required if Referenced Dose Reference Sequence (300C,0050) is sent.	*** not supported ***	*** not supported ***
>> Constraint Weight	(300A,0021)	3	Relative importance of satisfying constraint, where high values represent more important constraints.	*** not supported ***	*** not supported ***
>> Delivery Warning Dose	(300A,0022)	3	The dose (in Gy) which when reached or exceeded should cause some action to be taken.	*** not supported ***	*** not supported ***
>> Delivery Maximum Dose	(300A,0023)	3	The maximum dose (in Gy) which can be delivered to the dose reference.	*** not supported ***	*** not supported ***
>> Target Minimum Dose	(300A,0025)	3	Minimum permitted dose (in Gy) to Dose Reference if Dose Reference Type (300A,0020) of referenced Dose Reference is TARGET.	*** not supported ***	*** not supported ***
>> Target Prescription Dose	(300A,0026)	3	Prescribed dose (in Gy) to Dose Reference if Dose Reference Type (300A,0020) of referenced Dose Reference is TARGET.	*** not supported ***	*** not supported ***
>> Target Maximum Dose	(300A,0027)	3	Maximum permitted dose (in Gy) to Dose Reference if Dose Reference Type (300A,0020) of referenced Dose Reference is TARGET.	*** not supported ***	*** not supported ***

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
>> Target Underdose Volume Fraction	(300A,0028)	3	Maximum permitted fraction (in percent) of Target to receive less than the Target Prescription Dose (300A,0027) if Dose Reference Type (300A,0020) of referenced Dose Reference is TARGET and Dose Reference Structure Type (300A,0014) of referenced Dose Reference is VOLUME.	*** not supported ***	*** not supported ***
>> Organ at Risk Full-volume Dose	(300A,002A)	3	Maximum dose (in Gy) to entire Dose Reference if Dose Reference Type (300A,0020) of referenced Dose Reference is ORGAN_AT_RISK and Dose Reference Structure Type (300A,0014) of referenced Dose Reference is VOLUME.	*** not supported ***	*** not supported ***
>> Organ at Risk Limit Dose	(300A,002B)	3	Maximum permitted dose (in Gy) to any part of Dose Reference if Dose Reference Type (300A,0020) of referenced Dose Reference is ORGAN_AT_RISK and Dose Reference Structure Type (300A,0014) of referenced Dose Reference is VOLUME.	*** not supported ***	*** not supported ***
>> Organ at Risk Maximum Dose	(300A,002C)	3	Maximum dose (in Gy) to non-overdosed part of Dose Reference if Dose Reference Type (300A,0020) of referenced Dose Reference is ORGAN_AT_RISK and Dose Reference Structure Type (300A,0014) of referenced Dose Reference is VOLUME.	*** not supported ***	*** not supported ***
>> Organ at Risk Overdose Volume Fraction	(300A,002D)	3	Maximum permitted fraction (in percent) of Organ at Risk to receive more than the Organ at Risk Maximum Dose if Dose Reference Type (300A,0020) of referenced Dose Reference is ORGAN_AT_RISK and Dose Reference Structure Type (300A,0014) of referenced Dose Reference is VOLUME.	*** not supported ***	*** not supported ***
> Number of Fractions Planned	(300A,0078)	2	Total number of treatments (Fractions) prescribed for current Fraction Group.	Roundtrip supported	Roundtrip supported
> Number of Fraction Pattern Digits Per Day	(300A,0079)	3	Number of digits in Fraction Pattern (300A,007B) used to represent one day. See Note 2.	*** not supported ***	Roundtrip supported

IOD Details, RT Fraction Scheme – C.8.8.13

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
> Repeat Fraction Cycle Length	(300A,007A)	3	Number of weeks needed to describe treatment pattern. See Note 2.	*** not supported ***	Roundtrip supported
> Fraction Pattern	(300A,007B)	3	String of 0's (no treatment) and 1's (treatment) describing treatment pattern. Length of string is 7 x Number of Fraction Pattern Digits Per Day x Repeat Fraction Cycle Length. Pattern shall start on a Monday. See Note 2.	Roundtrip supported	Roundtrip supported
> Number of Beams	(300A,0080)	1	Number of Beams in current Fraction Group. If Number of Beams is greater than zero, Number of Brachy Application Setups (300A,00A0) shall equal zero.	Import only	Import only
> Referenced Beam Sequence	(300C,0004)	1C	Introduces sequence of treatment beams in current Fraction Group. Required if Number of Beams (300A,0080) is greater than zero. One or more items may be included in this sequence.	Roundtrip supported	Roundtrip supported
>> Referenced Beam Number	(300C,0006)	1C	Uniquely identifies Beam specified by Beam Number (300A,00C0) within Beam Sequence (300A,00B0) in RT Beams Module. Required if Referenced Beam Sequence (300C,0004) is sent.	Roundtrip supported	Roundtrip supported
>> Beam Dose Specification Point	(300A,0082)	3	Coordinates (x,y,z) of point at which Beam Dose is specified in the patient based coordinate system described in C.7.6.2.1.1 (mm). See Note 3.	Roundtrip supported	Roundtrip supported
>> Beam Dose	(300A,0084)	3	Dose (in Gy) at Beam Dose Specification Point (300A,0082) due to current Beam.	Roundtrip supported	Roundtrip supported
>> Beam Meterset	(300A,0086)	3	Machine setting to be delivered for current Beam, specified in Monitor Units (MU) or minutes as defined by Primary Dosimeter Unit (300A,00B3) (in RT Beams Module) for referenced Beam. See Note 4.	Roundtrip supported	Roundtrip supported

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
>> Maximum Treatment Time	(3249,XX00)	3	The maximum treatment time, which should not be exceeded. This items serves as a secondary safety limit besides the Beam Meterset value (300A,0086) itself. Units in [min].	Roundtrip supported	Roundtrip supported
> Number of Brachy Application Setups	(300A,00A0)	1	Number of Brachy Application Setups in current Fraction Group. If Number of Brachy Application Setups is greater than zero, Number of Beams (300A,0080) shall equal zero.	*** not supported ***	*** not supported ***
> Referenced Brachy Application Setup Sequence	(300C,000A)	1C	Introduces sequence of treatment Brachy Application Setups in current Fraction Group. Required if Number of Brachy Application Setups (300A,00A0) is greater than zero. One or more items may be included in this sequence.	*** not supported ***	*** not supported ***
>> Referenced Brachy Application Setup Number	(300C,000C)	1C	Uniquely identifies Brachy Application Setup specified by Brachy Application Setup Number (300A,0234) within Brachy Application Setup Sequence (300A,0230) in RT Brachy Application Setups Module. Required if Referenced Brachy Application Setup Sequence (300C,000A) is sent.	*** not supported ***	*** not supported ***
>> Brachy Application Setup Dose Specification Point	(300A,00A2)	3	Coordinates (x,y,z) of point in the patient based coordinate system described in C.7.6.2.1.1 at which Brachy Application Setup Dose (300A,00A4) is specified (mm).	*** not supported ***	*** not supported ***
>> Brachy Application Setup Dose	(300A,00A4)	3	Dose (in Gy) at Brachy Application Setup Dose Specification Point (300A,00A2) due to current Brachy Application Setup.	*** not supported ***	*** not supported ***
> Prescribed Dose per Fraction	(3269,XX00)	3		*** not supported ***	*** not supported ***
> Prescribed Percentage	(3269,XX01)	3		*** not supported ***	*** not supported ***
> Plan Normalization Factor	(3269,XX02)	3		*** not supported ***	*** not supported ***

C.2.11 RT Beams – C.8.8.14

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
Beam Sequence	(300A,00B0)	1	Introduces sequence of treatment beams for current RT Plan. One or more items may be included in this sequence.	Roundtrip supported	Roundtrip supported
> Beam Number	(300A,00C0)	1	Identification number of the Beam. The value of Beam Number (300A,00C0) shall be unique within the RT Plan in which it is created. See Note 1.	Roundtrip supported	Roundtrip supported
> Beam Name	(300A,00C2)	3	User-defined name for Beam. See Note 1.	Roundtrip supported	Roundtrip supported
> Beam Secondary Name	(3243,XX09)	3	User-defined secondary name for Beam.	Roundtrip supported	Roundtrip supported
> Beam Description	(300A,00C3)	3	User-defined description for Beam. See Note 1.	Roundtrip supported	Roundtrip supported
> Beam Type	(300A,00C4)	1	Motion characteristic of Beam. See Note 5. Enumerated Values: STATIC = All Control Point Sequence (300A,0111) attributes remain unchanged between consecutive pairs of control points with changing Cumulative Meterset Weight (300A,0134). DYNAMIC = One or more Control Point Sequence (300A,0111) attributes change between one or more consecutive pairs of control points with changing Cumulative Meterset Weight (300A,0134).	Roundtrip supported	Roundtrip supported
> Radiation Type	(300A,00C6)	2	Particle type of Beam. Defined Terms: PHOTON ELECTRON NEUTRON PROTON	Roundtrip supported	Roundtrip supported
> Primary Fluence Mode Sequence	(3002,0050)	3	Sequence defining whether the primary fluence of the treatment beam uses a non-standard fluence-shaping. Only a single Item shall be permitted in this sequence.	Roundtrip supported	Roundtrip supported

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
>u> Fluence Mode	(3002,0051)	1	Describes whether the fluence shaping is the standard mode for the beam or an alternate. Enumerated Values: STANDARD = Uses standard fluence-shaping NON_STANDARD = Uses a non-standard fluence-shaping mode	Roundtrip supported	Roundtrip supported
>> Fluence Mode ID	(3002,0052)	1C	Identifier for the specific fluence-shaping mode. Required if Fluence Mode (3002,0051) has value NON_STANDARD.	Roundtrip supported	Roundtrip supported
> Primary Fluence Mode Sequence (PRIVATE)	(3285,XX00)	3	See Primary Fluence Mode Sequence (3002,0050).	Roundtrip supported	Roundtrip supported
>> Fluence Mode (PRIVATE)	(3285,XX01)	1	See Fluence Mode (3002,0051).	Roundtrip supported	Roundtrip supported
>> Fluence Mode ID (PRIVATE)	(3285,XX02)	1C	See Fluence Mode ID (3002,0052).	Roundtrip supported	Roundtrip supported
> High-Dose Technique Type	(300A,00C7)	1C	Type of high-dose treatment technique. Defined Terms: NORMAL = Standard treatment TBI = Total Body Irradiation HDR = High Dose Rate Following defined term is supported additionally: SRS = Stereotactic Radiosurgery Required if treatment technique requires a dose that would normally require overriding of treatment machine safety controls.	Roundtrip supported	Roundtrip supported
> Treatment Machine Name	(300A,00B2)	2	User-defined name identifying treatment machine to be used for beam delivery. See Note 2.	Roundtrip supported	Roundtrip supported
> Manufacturer	(0008,0070)	3	Manufacturer of the equipment to be used for beam delivery.	Roundtrip supported	Roundtrip supported
> Institution Name	(0008,0080)	3	Institution where the equipment is located that is to be used for beam delivery.	Roundtrip supported	Roundtrip supported

IOD Details, RT Beams – C.8.8.14

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
> Institution Address	(0008,0081)	3	Mailing address of the institution where the equipment is located that is to be used for beam delivery.	*** not supported ***	*** not supported ***
> Institutional Department Name	(0008,1040)	3	Department in the institution where the equipment is located that is to be used for beam delivery.	Roundtrip supported	Roundtrip supported
> Manufacturer's Model Name	(0008,1090)	3	Manufacturer's model name of the equipment that is to be used for beam delivery.	Roundtrip supported	Roundtrip supported
> Device Serial Number	(0018,1000)	3	Manufacturer's serial number of the equipment that is to be used for beam delivery.	Roundtrip supported	Roundtrip supported
> Primary Dosimeter Unit	(300A,00B3)	3	Measurement unit of machine dosimeter. See C.8.8.14.1. Enumerated Values: MU = Monitor Unit MINUTE = minute	Roundtrip supported	Roundtrip supported
> Referenced Tolerance Table Number	(300C,00A0)	3	Uniquely identifies Tolerance Table specified by Tolerance Table Number (300A,0042) within Tolerance Table Sequence in RT Tolerance Tables Module. These tolerances are to be used for verification of treatment machine settings.	Roundtrip supported	Roundtrip supported
> Source-Axis Distance	(300A,00B4)	3	Radiation source to Gantry rotation axis distance of the equipment that is to be used for beam delivery (mm).	Roundtrip supported	Roundtrip supported
> Beam Limiting Device Sequence	(300A,00B6)	1	Introduces sequence of beam limiting device (collimator) jaw or leaf (element) sets. One or more items may be included in this sequence.	Roundtrip supported	Roundtrip supported

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
>> RT Beam Limiting Device Type	(300A,00B8)	1	Type of beam limiting device (collimator). Enumerated Values: X = symmetric jaw pair in IEC X direction Y = symmetric jaw pair in IEC Y direction ASYMX = asymmetric jaw pair in IEC X direction ASYMY = asymmetric pair in IEC Y direction MLCX = multileaf (multi-element) jaw pair in IEC X direction MLCY = multileaf (multi-element) jaw pair in IEC Y direction	Roundtrip supported	Roundtrip supported
>> Source to Beam Limiting Device Distance	(300A,00BA)	3	Radiation source to beam limiting device (collimator) distance of the equipment that is to be used for beam delivery (mm).	Roundtrip supported	Roundtrip supported
>> Number of Leaf/Jaw Pairs	(300A,00BC)	1	Number of leaf (element) or jaw pairs (equal to 1 for standard beam limiting device jaws).	Roundtrip supported	Roundtrip supported
>> Leaf Position Boundaries	(300A,00BE)	2C	Boundaries of beam limiting device (collimator) leaves (in mm) in IEC BEAM LIMITING DEVICE coordinate axis appropriate to RT Beam Limiting Device Type (300A,00B8), i.e. X-axis for MLCY, Y-axis for MLCX. Contains N+1 values, where N is the Number of Leaf/Jaw Pairs (300A,00BC), starting from Leaf (Element) Pair 1. Required if Beam Limiting Device Sequence (300A,00B6) is sent and RT Beam Limiting Device Type (300A,00B8) is MLCX or MLCY. See Note 3.	Roundtrip supported	Roundtrip supported
> Referenced Patient Setup Number	(300C,006A)	3	Uniquely identifies Patient Setup to be used for current beam, specified by Patient Setup Number (300A,0182) within Patient Setup Sequence of RT Patient Setup Module.	Roundtrip supported	Roundtrip supported
> Referenced Reference Image Sequence	(300C,0042)	3	Introduces sequence of reference images used for validation of current beam. One or more items may be included in this sequence.	Roundtrip supported	Roundtrip supported

IOD Details, RT Beams – C.8.8.14

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
>> Referenced SOP Class UID	(0008,1150)	1C	Uniquely identifies the referenced SOP Class. Required if Referenced Reference Image Sequence (300C,0042) is sent.	Roundtrip supported	Roundtrip supported
>> Referenced SOP Instance UID	(0008,1155)	1C	Uniquely identifies the referenced SOP Instance. Required if Referenced Reference Image Sequence (300C,0042) is sent.	Roundtrip supported	Roundtrip supported
>> Reference Image Number	(300A,00C8)	1C	Uniquely identifies Reference Image within Referenced Reference Image Sequence (300A,0042). Required if Referenced Reference Image Sequence (300A,0042) is sent.	Roundtrip supported	Roundtrip supported
>> Start Cumulative Meterset Weight	(300C,0008)	3	Cumulative Meterset Weight within current Beam at which image acquisition starts.	*** not supported ***	*** not supported ***
>> End Cumulative Meterset Weight	(300C,0009)	3	Cumulative Meterset Weight within current Beam at which image acquisition ends.	*** not supported ***	*** not supported ***
> Planned Verification Image Sequence	(300A,00CA)	3	Introduces sequence of planned verification images to be acquired during current beam. One or more items may be included in this sequence. See C.8.8.14.2.	Roundtrip supported	Roundtrip supported
>> Start Cumulative Meterset Weight	(300C,0008)	3	Cumulative Meterset Weight within current Beam at which image acquisition will start.	Roundtrip supported	Roundtrip supported
>> Meterset Exposure	(3002,0032)	3	Meterset duration over which image is to be acquired, specified in Monitor units (MU) or minutes as defined by Primary Dosimeter Unit (300A,00B3).	Roundtrip supported	*** not supported ***
>> End Cumulative Meterset Weight	(300C,0009)	3	Cumulative Meterset Weight within current Beam at which image acquisition will end.	*** not supported ***	*** not supported ***
>> RT Image Plane	(3002,000C)	3	Describes whether or not image plane is normal to beam axis. Enumerated Values: NORMAL = image plane normal to beam axis NON_NORMAL = image plane non-normal to beam axis	Roundtrip supported	Roundtrip supported

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
>> X-Ray Image Receptor Angle	(3002,000E)	3	X-Ray Image Receptor Angle i.e. orientation of IEC X-RAY IMAGE RECEPTOR coordinate system with respect to IEC GANTRY coordinate system (degrees). See C.8.8.14.3.	Roundtrip supported	Roundtrip supported
>> RT Image Orientation	(3002,0010)	3	The direction cosines of the first row and the first column with respect to the IEC XRAY IMAGE RECEPTOR coordinate system.	*** not supported ***	*** not supported ***
>> RT Image Position	(3002,0012)	3	The x and y coordinates (in mm) of the upper left hand corner of the image, in the IEC X-RAY IMAGE RECEPTOR coordinate system. This is the center of the first pixel transmitted.	Roundtrip supported	Roundtrip supported
>> RT Image SID	(3002,0026)	3	Radiation machine source to image plane distance (mm).	Roundtrip supported	Roundtrip supported

IOD Details, RT Beams – C.8.8.14

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
>> Imaging Device-Specific Acquisition Parameters	(300A,00CC)	3	User-specified device-specific parameters that describe how the imager will acquire the image.	Roundtrip supported	Roundtrip supported Type/quality used to acquire verification image. This field can have one of the following values: PortImageHighQuality Single port image optimized for image quality. PortImageLowDose Single port image optimized for low dose. PortImageContinuous Multiple port images acquired at highest possible rate. Start Cumulative Meterset Weight (300C,0008) must be 0. PortImageIntegrated Integrated port image with frames averaged during the entire beam on time.

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
>> Referenced Reference Image Number	(300C,0007)	3	Uniquely identifies Reference Image to which planned verification image is related, specified by Reference Image Number (300A,00C8) within Referenced Reference Image Sequence (300A,0042).	*** not supported ***	*** not supported ***
> Treatment Delivery Type	(300A,00CE)	3	Delivery Type of treatment. Defined Terms: TREATMENT = normal patient treatment SETUP = setup verification OPEN_PORTFILM = portal image acquisition with open field TRMT_PORTFILM = portal image acquisition with treatment port CONTINUATION = continuation of interrupted treatment	Roundtrip supported	Roundtrip supported
> Referenced Dose Sequence	(300C,0080)	3	Introduces sequence of related SOP Class/Instance pairs describing related instances of RT Dose (for grids, isodose curves, and named/unnamed point doses). One or more items may be included in this sequence.	Roundtrip supported	Roundtrip supported
>> Referenced SOP Class UID	(0008,1150)	1C	Uniquely identifies the referenced SOP Class. Required if Referenced Dose Sequence (300C,0080) is sent.	Roundtrip supported	Roundtrip supported
>> Referenced SOP Instance UID	(0008,1155)	1C	Uniquely identifies the referenced SOP Instance. Required if Referenced Dose Sequence (300C,0080) is sent.	Roundtrip supported	Roundtrip supported
> Number of Wedges	(300A,00D0)	1	Number of wedges associated with current Beam.	Roundtrip supported	Roundtrip supported
> Wedge Sequence	(300A,00D1)	1C	Introduces sequence of treatment wedges. Required if Number of Wedges (300A,00D0) is non-zero. One or more items may be included in this sequence.	Roundtrip supported	Roundtrip supported
>> Wedge Number	(300A,00D2)	1C	Identification number of the Wedge. The value of Wedge Number (300A,00D2) shall be unique within the Beam in which it is created. Required if Wedge Sequence (300A,00D1) is sent.	Roundtrip supported	Roundtrip supported

IOD Details, RT Beams – C.8.8.14

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
>> Wedge Type	(300A,00D3)	2C	Type of wedge (if any) defined for Beam. Required if Wedge Sequence (300A,00D1) is sent. Defined Terms: STANDARD = standard (static) wedge DYNAMIC = moving beam limiting device (collimator) jaw simulating wedge MOTORIZED = single wedge which can be removed from beam remotely	Roundtrip supported	Roundtrip supported
>> Wedge ID	(300A,00D4)	3	User-supplied identifier for Wedge.	Roundtrip supported	Roundtrip supported
>> Accessory Code	(300A,00F9)	3	An identifier for the accessory intended to be read by a device such as a bar-code reader.	Roundtrip supported	*** not supported ***
>> Wedge Angle	(300A,00D5)	2C	Nominal wedge angle (degrees). Required if Wedge Sequence (300A,00D1) is sent.	Roundtrip supported	Roundtrip supported
>> Wedge Factor	(300A,00D6)	2C	Nominal wedge factor under machine calibration conditions at the beam energy specified by the Nominal Beam Energy (300A,0114) of the first Control Point of the Control Point Sequence (300A,0111). Required if Wedge Sequence (300A,00D1) is sent.	Roundtrip supported	Roundtrip supported
>> Wedge Orientation	(300A,00D8)	2C	Orientation of wedge, i.e. orientation of IEC WEDGE FILTER coordinate system with respect to IEC BEAM LIMITING DEVICE coordinate system (degrees). Required if Wedge Sequence (300A,00D1) is sent.	Roundtrip supported	Roundtrip supported
>> Source to Wedge Tray Distance	(300A,00DA)	3	Radiation source to wedge tray attachment edge distance (in mm) for current wedge.	Roundtrip supported	Roundtrip supported
> Number of Compensators	(300A,00E0)	1	Number of compensators associated with current Beam.	Roundtrip supported	Import only.
> Total Compensator Tray Factor	(300A,00E2)	3	Compensator Tray transmission factor (between 0 and 1), at the beam energy specified by the Nominal Beam Energy (300A,0114) of the first Control Point of the Control Point Sequence (300A,0111).	*** not supported ***	Roundtrip supported

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
> Compensator Sequence	(300A,00E3)	1C	Introduces sequence of treatment compensators. Required if Number of Compensators (300A,00E0) is non-zero. One or more items may be included in this sequence.	Roundtrip supported	Roundtrip supported
>> Compensator Description	(300A,02EB)	3	User defined description for the compensator	*** not supported ***	*** not supported ***
>> Compensator Type	(300A,00EE)	3	Type of compensator (if any). Defined Terms: STANDARD = physical (static) compensator DYNAMIC = moving Beam Limiting Device (collimator) simulating physical compensator	Roundtrip supported	Roundtrip supported
>> Material ID	(300A,00E1)	2C	User-supplied identifier for material used to manufacture Compensator. Required if Number of Compensators (300A,00E0) is non-zero.	Roundtrip supported	Roundtrip supported
>> Compensator ID	(300A,00E5)	3	User-supplied identifier for compensator.	Roundtrip supported	Roundtrip supported
>> Accessory Code	(300A,00F9)	3	An identifier for the accessory intended to be read by a device such as a bar-code reader.	Roundtrip supported	Roundtrip supported
>> Source to Compensator Tray Distance	(300A,00E6)	2C	Radiation source to compensator tray attachment edge distance (in mm) for current compensator. Required if Compensator Sequence (300A,00E3) is sent.	Roundtrip supported	Roundtrip supported
>> Compensator Divergence	(300A,02E0)	3	Indicates presence or absence of geometrical divergence of the compensator. Enumerated Values: PRESENT = the compensator is shaped according to the beam geometrical divergence. ABSENT = the compensator is not shaped according to the beam geometrical divergence.	*** not supported ***	Roundtrip supported

IOD Details, RT Beams – C.8.8.14

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
>> Compensator Mounting Position	(300A,02E1)	3	Indicates on which side of the Compensator Tray the compensator is mounted. Enumerated Values: PATIENT_SIDE = the compensator is mounted on the side of the Compensator Tray which is towards the patient. SOURCE_SIDE = the compensator is mounted on the side of the Compensator Tray which is towards the radiation source. DOUBLE_SIDED = the compensator has a shaped (i.e. non-flat) surface on both sides of the Compensator Tray.	*** not supported ***	Roundtrip supported
>> Compensator Rows	(300A,00E7)	1C	Number of rows in the compensator. Required if Compensator Sequence (300A,00E3) is sent.	Roundtrip supported	Roundtrip supported
>> Compensator Columns	(300A,00E8)	1C	Number of columns in the compensator. Required if Compensator Sequence (300A,00E3) is sent.	Roundtrip supported	Roundtrip supported
>> Compensator Pixel Spacing	(300A,00E9)	1C	Physical distance (in mm) between the center of each pixel projected onto machine isocentric plane. Specified by a numeric pair - adjacent row spacing (delimiter) adjacent column spacing. Required if Compensator Sequence (300A,00E3) is sent.	Roundtrip supported	Roundtrip supported
>> Compensator Position	(300A,00EA)	1C	The x and y coordinates of the upper left hand corner (first pixel transmitted) of the compensator, projected onto the machine isocentric plane in the IEC BEAM LIMITING DEVICE coordinate system (mm). Required if Compensator Sequence (300A,00E3) is sent.	Roundtrip supported	Roundtrip supported

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
>> Compensator Transmission Data	(300A,00EB)	1C	<p>A data stream of the pixel samples which comprise the compensator, expressed as broad-beam transmission values (between 0 and 1) along a ray line passing through the pixel, at the beam energy specified by the Nominal Beam Energy (300A,0114) of the first Control Point of the Control Point Sequence (300A,0111). The order of pixels sent is left to right, top to bottom, i.e., the upper left pixel is sent first followed by the remainder of the first row , followed by the first pixel of the 2nd row, then the remainder of the 2nd row and so on) when viewed from the radiation source. Required if Compensator Sequence (300A,00E3) is sent and Material ID (300A,00E1) is zero- length. See C.8.8.14.10.</p> <p>Note: Compensator Transmission Data may not be properly encoded if Explicit-VR transfer syntax is used and the VL of this attribute exceeds 65534 bytes.</p>	Roundtrip supported	Roundtrip supported
>> Compensator Thickness Data	(300A,00EC)	1C	<p>A data stream of the pixel samples which comprise the compensator, expressed as thicknesses (in mm). The order of pixels sent is left to right, top to bottom, i.e., the upper left pixel is sent first followed by the remainder of the first row , followed by the first pixel of the 2nd row, then the remainder of the 2nd row and so on) when viewed from the radiation source. Required if Compensator Sequence (300A,00E3) is sent and Material ID (300A,00E1) is nonzero length. See C.8.8.14.9 and C.8.8.14.10.</p> <p>Note: Compensator Thickness Data may not be properly encoded if Explicit- VR transfer syntax is used and the VL of this attribute exceeds 65534 bytes.</p>	Roundtrip supported	Roundtrip supported

IOD Details, RT Beams – C.8.8.14

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
>> Source to Compensator Distance	(300A,02E2)	1C	A data stream of the pixel samples which comprise the distance from the radiation source to the compensator surface closest to the radiation source (in mm). The order of pixels sent is left to right, top to bottom (upper left pixel, followed by the remainder of row 1, followed by the remainder of the columns). Required if Compensator Sequence (300A,00E3) is sent, Material ID (300A,00E1) is non-zero length, and Compensator Mounting Position (300A,02E1) is DOUBLE_SIDED. See C.8.8.14.9.	Roundtrip supported	Roundtrip supported
> Number of Boli	(300A,00ED)	1	Number of boli associated with current Beam.	Roundtrip supported	Roundtrip supported
> Referenced Bolus Sequence	(300C,00B0)	1C	Introduces sequence of boli associated with Beam. Required if Number of Boli (300A,00ED) is non-zero. One or more items may be included in this sequence.	Roundtrip supported	Roundtrip supported
>> Referenced ROI Number	(3006,0084)	1C	Uniquely identifies ROI representing the Bolus specified by ROI Number (3006,0022) in Structure Set ROI Sequence (3006,0020) in Structure Set Module within RT Structure Set in Referenced Structure Set Sequence (300C,0060) in RT General Plan Module. Required if Referenced Bolus Sequence (300C,00B0) is sent.	Roundtrip supported	Roundtrip supported
>> Bolus ID	(300A,00DC)	3	User-supplied identifier for the Bolus.	*** not supported ***	*** not supported ***
>> Bolus Description	(300A,00DD)	3	User-defined description for the Bolus.	*** not supported ***	*** not supported ***
>> Accessory Code	(300A,00F9)	3	An identifier for the accessory intended to be read by a device such as a bar-code reader.	Roundtrip supported	Roundtrip supported
> Number of Blocks	(300A,00F0)	1	Number of shielding blocks associated with Beam.	Roundtrip supported	Roundtrip supported

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
> Total Block Tray Factor	(300A,00F2)	3	Total block tray transmission for all block trays (between 0 and 1) at the beam energy specified by the Nominal Beam Energy (300A,0114) of the first Control Point of the Control Point Sequence (300A,0111).	Roundtrip supported	Roundtrip supported
> Block Sequence	(300A,00F4)	1C	Introduces sequence of blocks associated with Beam. Required if Number of Blocks (300A,00F0) is non-zero. One or more items may be included in this sequence.	Roundtrip supported	Roundtrip supported
>> Block Tray ID	(300A,00F5)	3	User-supplied identifier for block tray.	Roundtrip supported	Roundtrip supported
>> Accessory Code	(300A,00F9)	3	An identifier for the accessory intended to be read by a device such as a bar-code reader.	Roundtrip supported	Roundtrip supported
>> Source to Block Tray Distance	(300A,00F6)	2C	Radiation Source to attachment edge of block tray assembly (mm). Required if Block Sequence (300A,00F4) is sent.	Roundtrip supported	Roundtrip supported
>> Block Type	(300A,00F8)	1C	Type of block. Required if Block Sequence (300A,00F4) is sent. See C.8.8.14.4. Enumerated Values: SHIELDING = blocking material is inside contour APERTURE = blocking material is outside contour	Roundtrip supported	Roundtrip supported
>> Block Divergence	(300A,00FA)	2C	Indicates presence or otherwise of geometrical divergence. Required if Block Sequence (300A,00F4) is sent. Enumerated Values: PRESENT = block edges are shaped for beam divergence ABSENT = block edges are not shaped for beam divergence	Roundtrip supported	Roundtrip supported
>> Block Mounting Position	(300A,00FB)	3	Indicates on which side of the Block Tray the block is mounted. Enumerated Values: PATIENT_SIDE = the block is mounted on the side of the Block Tray which is towards the patient. SOURCE_SIDE = the block is mounted on the side of the Block Tray which is towards the radiation source.	*** not supported ***	*** not supported ***

IOD Details, RT Beams – C.8.8.14

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
>> Block Number	(300A,00FC)	1C	Identification number of the Block. The value of Block Number (300A,00FC) shall be unique within the Beam in which it is created. Required if Block Sequence (300A,00F4) is sent.	Roundtrip supported	Roundtrip supported
>> Block Name	(300A,00FE)	3	User-defined name for block.	Roundtrip supported	Roundtrip supported
>> Material ID	(300A,00E1)	2C	User-supplied identifier for material used to manufacture Block. Required if Block Sequence (300A,00F4) is sent.	Roundtrip supported	Roundtrip supported
>> Block Thickness	(300A,0100)	2C	Physical thickness of block (in mm) parallel to radiation beam axis. Required if Block Sequence (300A,00F4) is sent and Material ID (300A,00E1) is non-zero length. See C.8.8.14.4.	Roundtrip supported	Roundtrip supported
>> Block Transmission	(300A,0102)	2C	Transmission through the block (between 0 and 1) at the beam energy specified by the Nominal Beam Energy (300A,0114) of the first Control Point of the Control Point Sequence (300A,0111). Required if Block Sequence (300A,00F4) is sent and Material ID (300A,00E1) is zero length. See C.8.8.14.4.	Roundtrip supported	Roundtrip supported
>> Block Number of Points	(300A,0104)	2C	Number of (x,y) pairs defining the block edge. Required if Block Sequence (300A,00F4) is sent.	Roundtrip supported	Roundtrip supported
>> Block Data	(300A,0106)	2C	A data stream of (x,y) pairs which comprise the block edge. The number of pairs shall be equal to Block Number of Points (300A,0104), and the vertices shall be interpreted as a closed polygon. Coordinates are projected onto the machine isocentric plane in the IEC BEAM LIMITING DEVICE coordinate system (mm). Required if Block Sequence (300A,00F4) is sent. See Note 4.	Roundtrip supported	Roundtrip supported
> Applicator Sequence	(300A,0107)	3	Introduces sequence of Applicators associated with Beam. Only a single item shall be permitted in this sequence.	Roundtrip supported	Roundtrip supported

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
>> Applicator ID	(300A,0108)	1C	User or machine supplied identifier for Applicator. Required if Applicator Sequence (300A,0107) is sent.	Roundtrip supported	Roundtrip supported
>> Accessory Code	(300A,00F9)	3	An identifier for the accessory intended to be read by a device such as a bar-code reader.	Roundtrip supported	Roundtrip supported
>> Applicator Type	(300A,0109)	1C	Type of Applicator. Required if Applicator Sequence (300A,0107) is sent. Defined Terms: ELECTRON_SQUARE = square electron applicator ELECTRON_RECT = rectangular electron applicator ELECTRON_CIRC = circular electron applicator ELECTRON_SHORT = short electron applicator ELECTRON_OPEN = open (dummy) electron applicator INTRAOPERATIVE = intraoperative (custom) applicator STEREOTACTIC = stereotactic applicator	Roundtrip supported	Roundtrip supported
>> Applicator Description	(300A,010A)	3	User-defined description for Applicator.	Roundtrip supported	Roundtrip supported
> General Accessory Sequence	(300A,0420)	3	Introduces a Sequence of General Accessories associated with this Beam. One or more items may be included in this sequence.	Roundtrip supported	Roundtrip supported
>> General Accessory Number	(300A,0424)	1	Identification Number of the General Accessory. The value shall be unique within the sequence.	Roundtrip supported	Roundtrip supported
>> General Accessory ID	(300A,0421)	1	User or machine supplied identifier for General Accessory.	Roundtrip supported	Roundtrip supported
>> General Accessory Description	(300A,0422)	3	User supplied description of General Accessory.	Roundtrip supported	Roundtrip supported

IOD Details, RT Beams – C.8.8.14

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
>> General Accessory Type	(300A,0423)	3	Specifies the type of accessory. Defined Terms: GRATICULE = Accessory tray with a radio-opaque grid IMAGE_DETECTOR = Image acquisition device positioned in the beam line RETICLE = Accessory tray with radio-transparent markers or grid	Roundtrip supported	Roundtrip supported
>> Accessory Code	(300A,00F9)	3	Machine-readable identifier for this accessory	Roundtrip supported	Roundtrip supported
>> Source to General Accessory Distance	(3291,XX00)	3	Radiation source to accessory distance of the equipment that is to be used for beam delivery (mm).	Roundtrip supported	Roundtrip supported
> Final Cumulative Meterset Weight	(300A,010E)	1C	Value of Cumulative Meterset Weight (300A,0134) for final Control Point in Control Point Sequence (300A,0111). Required if Cumulative Meterset Weight is non-null in Control Points specified within Control Point Sequence (300A,0111). See C.8.8.14.1.	Roundtrip supported	Roundtrip supported
> Number of Control Points	(300A,0110)	1	Number of control points in Beam.	Roundtrip supported	Roundtrip supported
> Control Point Sequence	(300A,0111)	1	Introduces sequence of machine configurations describing treatment beam. Two or more items may be included in this sequence. See C.8.8.14.5 and C.8.8.14.6.	Roundtrip supported	Roundtrip supported
>> Control Point Index	(300A,0112)	1C	Index of current Control Point, starting at 0 for first Control Point. Required if Control Point Sequence (300A,0111) is sent.	Roundtrip supported	Roundtrip supported
>> Cumulative Meterset Weight	(300A,0134)	2C	Cumulative weight to current control point. Cumulative Meterset Weight for the first item in Control Point Sequence shall always be zero. Cumulative Meterset Weight for the final item in Control Point Sequence shall always be equal to Final Cumulative Meterset Weight. Required if Control Point Sequence (300A,0111) is sent. See C.8.8.14.1.	Roundtrip supported	Roundtrip supported

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
>> Referenced Dose Reference Sequence	(300C,0050)	3	Introduces a sequence of Dose References for current Beam. One or more items may be included in this sequence.	Roundtrip supported	Roundtrip supported
>>> Referenced Dose Reference Number	(300C,0051)	1C	Uniquely identifies Dose Reference specified by Dose Reference Number (300A,0012) in Dose Reference Sequence (300A,0010) in RT Prescription Module. Required if Referenced Dose Reference Sequence (300C,0050) is sent.	Roundtrip supported	Roundtrip supported
>>> Cumulative Dose Reference Coefficient	(300A,010C)	2C	Coefficient used to calculate cumulative dose contribution from this Beam to the referenced Dose Reference at the current Control Point. Required if Referenced Dose Reference Sequence (300C,0050) is sent. See C.8.8.14.7.	Roundtrip supported	Roundtrip supported
>> Referenced Dose Sequence	(300C,0080)	1C	Sequence describing related instances of RT Dose (for grids, isodose curves, and named/unnamed point doses). One or more items may be included in this sequence. Required if RT Dose is being sent, and Dose Summation Type (3004,000A) equals CONTROL_POINT.	*** not supported ***	*** not supported ***
>>> Referenced SOP Class UID	(0008,1150)	1	Uniquely identifies the referenced SOP Class.	*** not supported ***	*** not supported ***
>>> Referenced SOP Instance UID	(0008,1155)	1	Uniquely identifies the referenced SOP Instance.	*** not supported ***	*** not supported ***
>> Nominal Beam Energy	(300A,0114)	3	Nominal Beam Energy at control point (MV/MeV).	Roundtrip supported	Roundtrip supported
>> Dose Rate Set	(300A,0115)	3	Dose Rate to be set on treatment machine for segment beginning at current control point (e.g. MU/min).	Roundtrip supported	Roundtrip supported

IOD Details, RT Beams – C.8.8.14

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
>> Wedge Position Sequence	(300A,0116)	3	A Sequence of Items describing Wedge Positions for the current control point. Required for first item of Control Point Sequence if Number of Wedges (300A,00D0) is non-zero, and in subsequent control points if Wedge Position (300A,0118) changes during Beam. See C.8.8.14.5. The number of items in this sequence shall equal the value of Number of Wedges (300A,00D0).	Roundtrip supported	Roundtrip supported
>>> Referenced Wedge Number	(300C,00C0)	1C	Uniquely references Wedge described by Wedge Number (300A,00D2) in Wedge Sequence (300A,00D1). Required if Wedge Position Sequence (300A,0116) is sent.	Roundtrip supported	Roundtrip supported
>>> Wedge Position	(300A,0118)	1C	Position of Wedge at current Control Point. Required if Wedge Position Sequence (300A,0116) is sent. Enumerated Values: IN OUT	Roundtrip supported	Roundtrip supported
>> Beam Limiting Device Position Sequence	(300A,011A)	1C	Introduces sequence of beam limiting device (collimator) jaw or leaf (element) positions. Required for first item of Control Point Sequence, or if Beam Limiting Device changes during Beam. One or more items may be included in this sequence.	Roundtrip supported	Roundtrip supported

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
>>> RT Beam Limiting Device Type	(300A,00B8)	1C	Type of beam limiting device (collimator). The value of this attribute shall correspond to RT Beam Limiting Device Type (300A,00B8) defined in an item of Beam Limiting Device Sequence (300A,00B6). Required if Beam Limiting Device Position Sequence (300A,011A) is sent. Enumerated Values: X = symmetric jaw pair in IEC X direction Y = symmetric jaw pair in IEC Y direction ASYMX = asymmetric jaw pair in IEC X direction ASYMY = asymmetric pair in IEC Y direction MLCX = multileaf (multi-element) jaw pair in IEC X direction MLCY = multileaf (multi-element) jaw pair in IEC Y direction	Roundtrip supported	Roundtrip supported
>>> Leaf/Jaw Positions	(300A,011C)	1C	Positions of beam limiting device (collimator) leaf (element) or jaw pairs (in mm) in IEC BEAM LIMITING DEVICE coordinate axis appropriate to RT Beam Limiting Device Type (300A,00B8), e.g. X- axis for MLCX, Y-axis for MLCY. Contains 2N values, where N is the Number of Leaf/Jaw Pairs (300A,00BC) in Beam Limiting Device Sequence (300A,00B6). Values shall be listed in IEC leaf (element) subscript order 101, 102, ... 1N, 201, 202, ... 2N. Required if Beam Limiting Device Position Sequence (300A,011A) is sent. See Note 2.	Roundtrip supported If values are not defined then 88888888 will be sent.	Roundtrip supported If values are not defined then 88888888 will be sent.
>> Gantry Angle	(300A,011E)	1C	Gantry angle of radiation source, i.e. orientation of IEC GANTRY coordinate system with respect to IEC FIXED REFERENCE coordinate system (degrees). Required for first item of Control Point Sequence, or if Gantry Angle changes during Beam.	Roundtrip supported If values are not defined then 88888888 will be sent.	Roundtrip supported If values are not defined then 88888888 will be sent.

IOD Details, RT Beams – C.8.8.14

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
>> Gantry Rotation Direction	(300A,011F)	1C	Direction of Gantry Rotation when viewing gantry from isocenter, for segment following Control Point. Required for first item of Control Point Sequence, or if Gantry Rotation Direction changes during Beam. See C.8.8.14.8. Enumerated Values: CW = clockwise CC = counter-clockwise NONE = no rotation	Roundtrip supported	Roundtrip supported
>> Gantry Pitch Angle	(300A,014A)	3	Gantry Pitch Angle. i.e. the rotation of the IEC GANTRY coordinate system about the X-axis of the IEC GANTRY coordinate system (degrees). If used, must be present for first item of Control Point Sequence, or if used and Gantry Pitch Rotation Angle changes during Beam, must be present.	*** not supported ***	*** not supported ***
>> Gantry Pitch Rotation Direction	(300A,014C)	3	Direction of Gantry Pitch Angle when viewing along the positive X-axis of the IEC GANTRY coordinate system, for segment following Control Point. If used, must be present for first item of Control Point Sequence, or if used and Gantry Pitch Rotation Direction changes during Beam, must be present. See C.8.8.14.8 and C.8.8.25.6.5. Enumerated Values: CW = clockwise CC = counter-clockwise NONE = no rotation	*** not supported ***	*** not supported ***
>> Beam Limiting Device Angle	(300A,0120)	1C	Beam Limiting Device angle, i.e. orientation of IEC BEAM LIMITING DEVICE coordinate system with respect to IEC GANTRY coordinate system (degrees). Required for first item of Control Point Sequence, or if Beam Limiting Device Angle changes during Beam.	Roundtrip supported	Roundtrip supported

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
>> Beam Limiting Device Rotation Direction	(300A,0121)	1C	Direction of Beam Limiting Device Rotation when viewing beam limiting device (collimator) from radiation source, for segment following Control Point. Required for first item of Control Point Sequence, or if Beam Limiting Device Rotation Direction changes during Beam. See C.8.8.14.8. Enumerated Values: CW = clockwise CC = counter-clockwise NONE = no rotation	Roundtrip supported	Roundtrip supported
>> Patient Support Angle	(300A,0122)	1C	Patient Support angle, i.e. orientation of IEC PATIENT SUPPORT (turntable) coordinate system with respect to IEC FIXED REFERENCE coordinate system (degrees). Required for first item of Control Point Sequence, or if Patient Support Angle changes during Beam.	Roundtrip supported	Roundtrip supported
>> Patient Support Rotation Direction	(300A,0123)	1C	Direction of Patient Support Rotation when viewing table from above, for segment following Control Point. Required for first item of Control Point Sequence, or if Patient Support Rotation Direction changes during Beam. See C.8.8.14.8. Enumerated Values: CW = clockwise CC = counter-clockwise NONE = no rotation	Roundtrip supported	Roundtrip supported
>> Table Top Eccentric Axis Distance	(300A,0124)	3	Distance (positive) from the IEC PATIENT SUPPORT vertical axis to the IEC TABLE TOP ECCENTRIC vertical axis (mm).	Roundtrip supported	Roundtrip supported
>> Table Top Eccentric Angle	(300A,0125)	1C	Table Top (non-isocentric) angle, i.e. orientation of IEC TABLE TOP ECCENTRIC coordinate system with respect to IEC PATIENT SUPPORT coordinate system (degrees). Required for first item of Control Point Sequence, or if Table Top Eccentric Angle changes during Beam.	Roundtrip supported	Roundtrip supported

IOD Details, RT Beams – C.8.8.14

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
>> Table Top Eccentric Rotation Direction	(300A,0126)	1C	Direction of Table Top Eccentric Rotation when viewing table from above, for segment following Control Point. Required for first item of Control Point Sequence, or if Table Top Eccentric Rotation Direction changes during Beam. See C.8.8.14.8. Enumerated Values: CW = clockwise CC = counter-clockwise NONE = no rotation	Roundtrip supported	Roundtrip supported
>> Patient Support Pitch Angle	(300A,0140)	1C	Table Top Pitch Angle, i.e. the rotation of the IEC TABLE TOP coordinate system about the X-axis of the IEC TABLE TOP coordinate system (degrees). If required by treatment delivery device, shall be present for first item of Control Point Sequence. If required by treatment delivery device and if Table Top Pitch Angle changes during Beam, shall be present in all subsequent items of Control Point Sequence. See C.8.8.25.6.2.	*** not supported ***	*** not supported ***
>> Patient Support Pitching Direction	(300A,0142)	1 C	Direction of Table Top Pitch Rotation when viewing the table along the positive X-axis of the IEC TABLE TOP coordinate system, for segment following Control Point. If required by treatment delivery device, shall be present for first item of Control Point Sequence. If required by treatment delivery device and if Table Top Pitch Rotation Direction changes during Beam, shall be present in all subsequent items of Control Point Sequence. See C.8.8.14.8 and C.8.8.25.6.2. Enumerated Values: CW = clockwise CC = counter-clockwise NONE = no rotation	*** not supported ***	*** not supported ***

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
>> Patient Support Roll Angle	(300A,0144)	1C	Table Top Roll Angle, i.e. the rotation of the IEC TABLE TOP coordinate system about the IEC Y-axis of the IEC TABLE TOP coordinate system (degrees). If required by treatment delivery device, shall be present for first item of Control Point Sequence. If required by treatment delivery device and if Table Top Roll Angle changes during Beam, shall be present in all subsequent items of Control Point Sequence. See C.8.8.25.6.2.	*** not supported ***	*** not supported ***
>> Patient Support Rolling Direction	(300A,0146)	1C	Direction of Table Top Roll Rotation when viewing the table along the positive Y-axis of the IEC TABLE TOP coordinate system, for segment following Control Point. If required by treatment delivery device, shall be present for first item of Control Point Sequence. If required by treatment delivery device and if Table Top Roll Rotation Direction changes during Beam, shall be present in all subsequent items of Control Point Sequence. See C.8.8.14.8 and C.8.8.25.6.2. Enumerated Values: CW = clockwise CC = counter-clockwise NONE = no rotation	*** not supported ***	*** not supported ***
>> Table Top Vertical Position	(300A,0128)	2C	Table Top Vertical position in IEC TABLE TOP coordinate system (mm). Required for first item of Control Point Sequence, or if Table Top Vertical Position changes during Beam. See C.8.8.14.6.	Roundtrip supported	Roundtrip supported
>> Table Top Longitudinal Position	(300A,0129)	2C	Table Top Longitudinal position in IEC TABLE TOP coordinate system (mm). Required for first item of Control Point Sequence, or if Table Top Longitudinal Position changes during Beam. See C.8.8.14.6.	Roundtrip supported	Roundtrip supported

IOD Details, RT Beams – C.8.8.14

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
>> Table Top Lateral Position	(300A,012A)	2C	Table Top Lateral position in IEC TABLE TOP coordinate system (mm). Required for first item of Control Point Sequence, or if Table Top Lateral Position changes during Beam. See C.8.8.14.6.	Roundtrip supported	Roundtrip supported
>> Virtual SAD	(3243,XX1A)	3	The virtual SAD for this control point. This SAD denotes the physical focus of the beam if it is different than the nominal Source Axis Distance (300A,00B4).	*** not supported ***	*** not supported ***
>> Table Top Pitch Angle	(300A,0140)	3	Table Top Pitch Angle, i.e. the rotation of the IEC TABLE TOP coordinate system about the X-axis of the IEC TABLE TOP coordinate system (degrees). If required by treatment delivery device, shall be present for first item of Control Point Sequence. If required by treatment delivery device and if Table Top Pitch Angle changes during Beam, shall be present in all subsequent items of Control Point Sequence	Beam will be valid if the tag is not available or has '0' (zero) value. For non-zero values, beam will be marked as invalid.	*** not supported ***
>> Table Top Pitch Rotation Direction	(300A,0142)	1C	Direction of Table Top Pitch Rotation when viewing the table along the positive X-axis of the IEC TABLE TOP coordinate system, for segment following Control Point. If required by treatment delivery device, shall be present for first item of Control Point Sequence. If required by treatment delivery device and if Table Top Pitch Rotation Direction changes during Beam, shall be present in all subsequent items of Control Point Sequence. See C.8.8.14.8 and C.8.8.25.6.2. Enumerated Values: CW = clockwise CC = counter-clockwise NONE = no rotation	Beam will be valid if the tag is not available or has any value. This value will be read and ignored.	*** not supported ***

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
>> Table Top Roll Angle	(300A,0144)	1C	Table Top Roll Angle, i.e. the rotation of the IEC TABLE TOP coordinate system about the IEC Y-axis of the IEC TABLE TOP coordinate system (degrees). If required by treatment delivery device, shall be present for first item of Control Point Sequence. If required by treatment delivery device and if Table Top Roll Angle changes during Beam, shall be present in all subsequent items of Control Point Sequence	Beam will be valid if the tag is not available or has '0' (zero) value. For non-zero values, beam will be marked as invalid.	*** not supported ***
>> Table Top Roll Rotation Direction	(300A,0146)	1C	Direction of Table Top Roll Rotation when viewing the table along the positive Y-axis of the IEC TABLE TOP coordinate system, for segment following Control Point. If required by treatment delivery device, shall be present for first item of Control Point Sequence. If required by treatment delivery device and if Table Top Roll Rotation Direction changes during Beam, shall be present in all subsequent items of Control Point Sequence. See C.8.8.14.8 and C.8.8.25.6.2. Enumerated Values: CW = clockwise CC = counter-clockwise NONE = no rotation	Beam will be valid if the tag is not available or has any value. This value will be read and ignored.	*** not supported ***
>> Isocenter Position	(300A,012C)	2C	Isocenter coordinates (x,y,z) in the patient based coordinate system described in C.7.6.2.1.1 (mm). Required for first item of Segment Control Point Sequence, or if Segment Isocenter Position changes during Beam.	Roundtrip supported	Roundtrip supported
>> Surface Entry Point	(300A,012E)	3	Patient surface entry point coordinates (x,y,z) in the patient based coordinate system described in C.7.6.2.1.1 (mm).	*** not supported ***	*** not supported ***
>> Source to Surface Distance	(300A,0130)	3	Source to Patient Surface distance (mm).	Roundtrip supported	Roundtrip supported

IOD Details, Approval – C.8.8.16

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
>> Referenced SOP Class UID	(0008,1150)	1	Uniquely identifies the referenced SOP Class.	*** not supported ***	*** not supported ***
>> Referenced SOP Instance UID	(0008,1155)	1	Uniquely identifies the referenced SOP Instance.	*** not supported ***	*** not supported ***

C.2.12 Approval – C.8.8.16

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
Approval Status	(300E,0002)	1	Approval status at the time the SOP Instance was created. Enumerated Values: APPROVED = Reviewer recorded that object met an implied criterion UNAPPROVED = No review of object has been recorded REJECTED = Reviewer recorded that object failed to meet an implied criterion	Roundtrip supported	Roundtrip supported
Review Date	(300E,0004)	2C	Date on which object was reviewed. Required if Approval Status (300E,0002) is APPROVED or REJECTED.	Roundtrip supported	Roundtrip supported
Review Time	(300E,0005)	2C	Time at which object was reviewed. Required if Approval Status (300E,0002) is APPROVED or REJECTED.	Roundtrip supported	Roundtrip supported
Reviewer Name	(300E,0008)	2C	Name of person who reviewed object. Required if Approval Status (300E,0002) is APPROVED or REJECTED.	Roundtrip supported	Roundtrip supported

C.2.13 SOP Common – C.12.1

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
SOP Class UID	(0008,0016)	1	Uniquely identifies the SOP Class. See C.12.1.1.1 for further explanation. See also PS 3.4.	Roundtrip supported	Roundtrip supported
SOP Instance UID	(0008,0018)	1	Uniquely identifies the SOP Instance. See C.12.1.1.1 for further explanation. See also PS 3.4.	Roundtrip supported	Roundtrip supported
Specific Character Set	(0008,0005)	1C	Character Set that expands or replaces the Basic Graphic Set. Required if an expanded or replacement character set is used. See C.12.1.1.2 for Defined Terms.	Roundtrip supported	Roundtrip supported
Instance Creation Date	(0008,0012)	3	Date the SOP Instance was created.	Roundtrip supported	Roundtrip supported
Instance Creation Time	(0008,0013)	3	Time the SOP Instance was created.	Roundtrip supported	Roundtrip supported
Instance Creator UID	(0008,0014)	3	Uniquely identifies device which created the SOP Instance.	Roundtrip supported	Roundtrip supported
Related General SOP Class UID	(0008,001A)	3	Uniquely identifies a Related General SOP Class for the SOP Class of this Instance. See PS 3.4.	*** not supported ***	*** not supported ***
Original Specialized SOP Class UID	(0008,001B)	3	The SOP Class in which the Instance was originally encoded, but which has been replaced during a fall-back conversion to the current Related General SOP Class. See PS 3.4.	*** not supported ***	*** not supported ***
Coding Scheme Identification Sequence	(0008,0110)	3	Sequence of items that map values of Coding Scheme Designator (0008,0102) to an external coding system registration, or to a private or local coding scheme. One or more items may be present in the sequence.	*** not supported ***	*** not supported ***
> Coding Scheme Designator	(0008,0102)	1	The value of a Coding Scheme Designator, used in this SOP Instance, which is being mapped.	*** not supported ***	*** not supported ***

IOD Details, SOP Common – C.12.1

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
> Coding Scheme Registry	(0008,0112)	1C	The name of the external registry where further definition of the identified coding scheme may be obtained. Required if coding scheme is registered. Defined term: HL7	*** not supported ***	*** not supported ***
> Coding Scheme UID	(0008,010C)	1C	The coding scheme UID identifier. Required if coding scheme is identified by an ISO 8824 object identifier compatible with the UI VR.	*** not supported ***	*** not supported ***
> Coding Scheme External ID	(0008,0114)	2C	The coding scheme identifier as defined in an external registry. Required if coding scheme is registered and Coding Scheme UID (0008,010C) is not present.	*** not supported ***	*** not supported ***
> Coding Scheme Name	(0008,0115)	3	The coding scheme full common name	*** not supported ***	*** not supported ***
> Coding Scheme Version	(0008,0103)	3	The coding scheme version associated with the Coding Scheme Designator (0008,0102).	*** not supported ***	*** not supported ***
> Responsible Organization	(0008,0116)	3	Name of the organization responsible for the Coding Scheme. May include organizational contact information.	*** not supported ***	*** not supported ***

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
Timezone Offset From UTC	(0008,0201)	3	<p>Contains the offset from UTC to the timezone for all DA and TM Attributes present in this SOP Instance. Encoded as an ASCII string in the format "&ZZZZ". The components of this string, from left to right, are & = "+" or "-", and ZZZZ = Hours and Minutes of offset.</p> <p>Notes:</p> <ol style="list-style-type: none"> 1. This encoding is the same as described in PS 3.5 for the DT Value Representation. 2. This Attribute does not apply to values with a DT Value Representation, which may contain an explicitly encoded timezone. 3. The corrected time may cross a 24 hour boundary. For example, if Local Time = 1.00 a.m. and Offset = +0200, then UTC = 11.00 p.m. (23.00) the day before. 4. The "+" sign may not be omitted. Time earlier than UTC is expressed as a negative offset. <p>Note:</p> <p>For example: UTC = 5.00 a.m. Local Time = 3.00 a.m. Offset = -0200 The local timezone offset is undefined if this Attribute is absent.</p>	*** not supported ***	*** not supported ***
Contributing Equipment Sequence	(0018,A001)	3	Sequence of Items containing descriptive attributes of related equipment which has contributed to the acquisition, creation or modification of the composite instance. One or more Items may be included in this Sequence. See C.12.1.1.5 for further explanation.	*** not supported ***	*** not supported ***
> Purpose of Reference Code Sequence	(0040,A170)	1	Describes the purpose for which the related equipment is being reference. Only a single Item shall be permitted in this sequence. See C.12.1.1.5 for further explanation.	*** not supported ***	*** not supported ***
>> Code Value	(0008,0100)	1C	See Section 8.1. Required if a sequence item is present.	*** not supported ***	*** not supported ***

IOD Details, SOP Common – C.12.1

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
>> Coding Scheme Designator	(0008,0102)	1C	See Section 8.2. Required if a sequence item is present.	*** not supported ***	*** not supported ***
>> Coding Scheme Version	(0008,0103)	1C	See Section 8.2. Required if a sequence item is present and the value of Coding Scheme Designator (0008,0102) is not sufficient to identify the Code Value (0008,0100) unambiguously.	*** not supported ***	*** not supported ***
>> Code Meaning	(0008,0104)	1C	See Section 8.3. Required if a sequence item is present.	*** not supported ***	*** not supported ***
> Manufacturer	(0008,0070)	1	Manufacturer of the equipment that contributed to the composite instance.	*** not supported ***	*** not supported ***
> Institution Name	(0008,0080)	3	Institution where the equipment that contributed to the composite instance is located.	*** not supported ***	*** not supported ***
> Institution Address	(0008,0081)	3	Address of the institution where the equipment that contributed to the composite instance is located.	*** not supported ***	*** not supported ***
> Station Name	(0008,1010)	3	User defined name identifying the machine that contributed to the composite instance.	*** not supported ***	*** not supported ***
> Institutional Department Name	(0008,1040)	3	Department in the institution where the equipment that contributed to the composite instance is located.	*** not supported ***	*** not supported ***
> Manufacturer's Model Name	(0008,1090)	3	Manufacturer's model name of the equipment that contributed to the composite instance.	*** not supported ***	*** not supported ***
> Device Serial Number	(0018,1000)	3	Manufacturer's serial number of the equipment that contributed to the composite instance.	*** not supported ***	*** not supported ***
> Software Version(s)	(0018,1020)	3	Manufacturer's designation of the software version of the equipment that contributed to the composite instance.	*** not supported ***	*** not supported ***
> Spatial Resolution	(0018,1050)	3	The inherent limiting resolution in mm of the acquisition equipment for high contrast objects for the data gathering and reconstruction technique chosen. If variable across the images of the series, the value at the image center.	*** not supported ***	*** not supported ***

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
> Date of Last Calibration	(0018,1200)	3	Date when the image acquisition device calibration was last changed in any way. Multiple entries may be used for additional calibrations at other times. See C.7.5.1.1.1 for further explanation.	*** not supported ***	*** not supported ***
> Time of Last Calibration	(0018,1201)	3	Time when the image acquisition device calibration was last changed in any way. Multiple entries may be used. See C.7.5.1.1.1 for further explanation.	*** not supported ***	*** not supported ***
> Contribution Date Time	(0018,A002)	3	The Date & Time when the equipment contributed to the composite instance.	*** not supported ***	*** not supported ***
> Contribution Description	(0018,A003)	3	Description of the contribution the equipment made to the composite instance.	*** not supported ***	*** not supported ***
Instance Number	(0020,0013)	3	A number that identifies this Composite object instance.	*** not supported ***	*** not supported ***

IOD Details, SOP Common – C.12.1

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
SOP Instance Status	(0100,0410)	3	<p>A flag that indicates the storage status of the SOP Instance. Not Specified (NS) implies that this SOP Instance has no special storage status, and hence no special actions need be taken. Original (OR) implies that this is the primary SOP instance for the purpose of storage, but that it has not yet been authorized for diagnostic use. Authorized Original (AO) implies that this is the primary SOP instance for the purpose of storage, which has been authorized for diagnostic use. Any copies of an Authorized Original should be given the status of Authorized Copy. Authorized Copy (AC) implies that this is a copy of an Authorized Original SOP Instance.</p> <p>Enumerated Values: NS, OR, AO, AC</p> <p>Note: Proper use of these flags is specified in Security Profiles. Implementations that do not conform to such Security Profiles may not necessarily handle these flags properly.</p>	*** not supported ***	*** not supported ***
SOP Authorization Date and Time	(0100,0420)	3	The date and time when the SOP Instance Status (0100,0410) was set to AO.	*** not supported ***	*** not supported ***
SOP Authorization Comment	(0100,0424)	3	Any comments associated with the setting of the SOP Instance Status (0100,0410) to AO.	*** not supported ***	*** not supported ***
Authorization Equipment Certification Number	(0100,0426)	3	The certification number issued to the Application Entity that set the SOP Instance Status (0100,0410) to AO.	*** not supported ***	*** not supported ***
MAC Parameters Sequence	(4FFE,0001)	3	A sequence of one or more items that describe the parameters used to calculate a MAC for use in Digital Signatures.	*** not supported ***	*** not supported ***
> MAC ID Number	(0400,0005)	1	A number used to identify this MAC Parameters Sequence item.	*** not supported ***	*** not supported ***

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
> MAC Calculation Transfer Syntax UID	(0400,0010)	1	The Transfer Syntax UID used to encode the values of the Data Elements included in the MAC calculation. Only Transfer Syntaxes that explicitly include the VR and use Little Endian encoding shall be used. Notes: Certain Transfer Syntaxes, particularly those that are used with compressed data, allow the fragmentation of the pixel data to change. If such fragmentation changes, Digital Signatures generated with such Transfer Syntaxes could become invalid.	*** not supported ***	*** not supported ***
> MAC Algorithm	(0400,0015)	1	The algorithm used in generating the MAC to be encrypted to form the Digital Signature. Defined Terms: RIPMD160 MD5 SHA1. Note: Digital Signature Security Profiles (see PS 3.15) may require the use of a restricted subset of these terms.	*** not supported ***	*** not supported ***
> Data Elements Signed	(0400,0020)	1	A list of Data Element Tags in the order they appear in the Data Set which identify the Data Elements used in creating the MAC for the Digital Signature. See Section C.12.1.1.3.1.1.	*** not supported ***	*** not supported ***
Digital Signatures Sequence	(FFFA,FFFA)	3	Sequence holding one or more Digital Signatures.	*** not supported ***	*** not supported ***
> MAC ID Number	(0400,0005)	1	A number used to identify which MAC Parameters Sequence item was used in the calculation of this Digital Signature.	*** not supported ***	*** not supported ***
> Digital Signature UID	(0400,0100)	1	A UID that can be used to uniquely reference this signature.	*** not supported ***	*** not supported ***

IOD Details, SOP Common – C.12.1

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
> Digital Signature DateTime	(0400,0105)	1	The date and time the Digital Signature was created. The time shall include an offset (i.e., time zone indication) from Coordinated Universal Time. Note: This is not a certified timestamp, and hence is not completely verifiable. An application can compare this date and time with those of other signatures and the validity date of the certificate to gain confidence in the veracity of this date and time.	*** not supported ***	*** not supported ***
> Certificate Type	(0400,0110)	1	The type of certificate used in (0400,0115). Defined Term: X509_1993_SIG Note: Digital Signature Security Profiles (see PS 3.15) may require the use of a restricted subset of these terms.	*** not supported ***	*** not supported ***
> Certificate of Signer	(0400,0115)	1	A certificate that holds the identity of the entity producing this Digital Signature, that entity's public key or key identifier, and the algorithm and associated parameters with which that public key is to be used. Algorithms allowed are specified in Digital Signature Security Profiles (see PS 3.15). Notes: 1. As technology advances, additional encryption algorithms may be allowed in future versions. Implementations should take this possibility into account. 2. When symmetric encryption is used, the certificate merely identifies which key was used by which entity, but not the actual key itself. Some other means (e.g., a trusted third party) must be used to obtain the key.	*** not supported ***	*** not supported ***
> Signature	(0400,0120)	1	The MAC generated as described in Section 12.2.1.1 and encrypted using the algorithm, parameters, and private key associated with the Certificate of the Signer (0400,0115). See Section C.12.1.1.3.1.2.	*** not supported ***	*** not supported ***

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
> Certified Timestamp Type	(0400,0305)	1C	The type of certified timestamp used in the Certified Timestamp (0400,0310) Attribute. Required if Certified Timestamp (0400,0310) is present. Defined Terms: CMS_TSP û Internet X.509 Public Key Infrastructure Time Stamp Protocol Note: Digital Signature Security Profiles (see PS 3.15) may require the use of a restricted subset of these terms.	*** not supported ***	*** not supported ***
> Certified Timestamp	(0400,0310)	3	A certified timestamp of the Digital Signature (0400,0120) Attribute Value, which shall be obtained when the Digital Signature is created. See Section C.12.1.1.3.1.3.	*** not supported ***	*** not supported ***
Encrypted Attributes Sequence	(0400,0500)	1C	Sequence of Items containing encrypted DICOM data. One or more Items shall be present. Required if application level confidentiality is needed and certain recipients are allowed to decrypt all or portions of the Encrypted Attributes Data Set. See C.12.1.1.4.1.	*** not supported ***	*** not supported ***
> Encrypted Content Transfer Syntax UID	(0400,0510)	1	Transfer Syntax used to encode the encrypted content. Only Transfer Syntaxes that explicitly include the VR and use Little Endian encoding shall be used.	*** not supported ***	*** not supported ***
> Encrypted Content	(0400,0520)	1	Encrypted data. See C.12.1.1.4.2.	*** not supported ***	*** not supported ***
HL7 Structured Document Reference Sequence	(0040,A390)	1C	Sequence of items defining mapping and/or access mechanism for HL7 Structured Documents referenced from the current SOP Instance. One or more Items may be included in this sequence. See C.12.1.1.6. Required if HL7 Structured Documents are referenced within the Instance.	*** not supported ***	*** not supported ***
> Referenced SOP Class UID	(0008,1150)	1	Unique identifier for the class of HL7 Structured Document.	*** not supported ***	*** not supported ***
> Referenced SOP Instance UID	(0008,1155)	1	Unique identifier for the HL7 Structured Document as used in DICOM instance references.	*** not supported ***	*** not supported ***

IOD Details, Extended Interface – Private

Attribute Name	Tag	Type	Attribute Description	TXA v2.5	4DITC v13.0
> HL7 Instance Identifier	(0040,E001)	1	Instance Identifier of the referenced HL7 Structured Document, encoded as a UID (OID or UUID), concatenated with a caret ("^") and Extension value (if Extension is present in Instance Identifier).	*** not supported ***	*** not supported ***
> Retrieve URI	(0040,E010)	3	Retrieval access path to HL7 Structured Document. Includes fully specified scheme, authority, path, and query in accordance with RFC 2396	*** not supported ***	*** not supported ***

C.2.14 Extended Interface – Private

Attribute Name	Tag	Type	Attribute Description	TxA v2.5	4DITC v13.0
Extended Interface Format	(3253,XX02)	1	Identifier string defining format of Extended Interface Data (3253,xx00). Applications should be able to unambiguously map this string to an XML schema definition.	Roundtrip supported	Roundtrip supported
Extended Interface Data	(3253,XX00)	1	Contains private extensions as an XML stream. Schema of XML is defined by Extended Interface Format (3253,xx02).	Roundtrip supported	Roundtrip supported
Extended Interface Length	(3253,XX01)	1	Length of XML stream contained in Extended Interface Data (3253,xx00). Usually is equal to attribute length of Extended Interface Data (3253,xx00) if length is even and is one less than attribute length if length is odd.	Roundtrip supported	Roundtrip supported

Appendix D **Extended Interface**

The following IODs have private Attributes containing an XML data structure for transporting structured non-DICOM data:

- RT Plan
- RT Beams Treatment Record

The following sections specify Attributes containing the XML data and describe the structure of the XML data.

D.1 RT Plan

The XML data structure for RT Plan IODs is contained in private Extended Interface Module which is optional within RT Plan IOD.

The structure of the XML data structure is described in the following table.

Column “Operational Mode” indicates the presence for certain XML nodes depending of the applications Operational Mode.

Legend for column “Operational Mode”:

- ✓ Attribute supported
- ✘ Attribute not supported
- 1) Present for Block, Compensator and empty Trays
- 1)* Present for empty Trays

Attributes not supported anymore in the Extended Interface XML data are covered by standard DICOM attributes.

Extended Interface, Extended Interface – Private

Node Name	Occurrence		Data Type	Node Description	Operational Mode	
	Min	Max			VMS Console System 6.5	VMS Console System 8.8 / QA
ExtendedVAPlanInterface	0	1			✓	✓
> Beams	0	1			✓	✓
>> Beam	0	∞			✓	✓
>>> ReferencedBeamNumber	1	1	int	Beam identifier	✓	✓
>>>> BeamExtension	1	1		Additional items provided from Vision to expand the features of RT Beams.	✓	✓
>>>>> FieldType	1	1	string	TREATMENT or SETUP	✓	*
>>>>> RelatedTreatBeamNumber	0	1	int	Relation from the image beams to the treatment and/or setup beams.	✓	✓
>>>>> FieldOrder	1	1	int	Order in which the fields are shown	✓	✓
>>>>> GantryRtnExtendedStart	0	1	int	When true, gantry angle position is in the extended range, which means it has an over travel (a Gantry can move most typical 400' and not only 360').	✓	✓
>>>>> GantryRtnExtendedStop	0	1	int	When true, gantry angle position is in the extended range, which means it has an over travel (a Gantry can move most typical 400' and not only 360').	✓	✓
>>>>> MUSubtraction	0	1	int	Although the extended interface contains the MUSubtraction attribute, it is not used in TXA.	✓	✓
>>>>> FieldSetupPhotos	0	1			✓	✓
>>>>>> FieldSetupPhoto	0	2		Two setup photos max	✓	✓
>>>>>>> SetupPhotoNumber	1	1	int	Increasing number of setup photos. The value has to start from 1 and up.	✓	✓
>>>>>>>> SetupPhotoFormat	1	1	string	The format of the pixel information. Supported values are 'JPG' and 'BMP'	✓	✓
>>>>>>>>> SetupPhotoPicture	1	1	hex binary	Pixel information of the photo in the corresponding format.	✓	✓
>>>>>>>>>> PhotoModified	1	1	string	Photo has been modified. PhotoModified may have 'true' or 'false'	✓	✓
>>>>> CustomAddOns	0	1			✓	*
>>>>>> CustomAddOn	0	4			1)	*
>>>>>>>> CustomAddOnType	1	1	string	Three Add On Type to choose from: BLOCK COMPENSATOR TRAY	1)	*

Extended Interface, Extended Interface – Private

>>>>> CustomCode	0	1	int	Codes for accessory which may be custom made or factory made (in that case the internal code in equal the custom code.)	1)	*
>>>>> ReferencedAddOnNumber	0	1	int	Reference to the identification number of the Block or Compensator.	1)	*
>>>>> TraySpecification	0	1		In case the CustomAddOn is a tray, it gets reported back through this node	1)*	*
>>>>>> TrayID	1	1	string	User-supplied identifier for tray. Max length is 16 characters.	1)*	*
>>>>>> SourceTrayDistance	0	1	int	The distance from source to slot. This information is needed to distinguish the slot	1)*	*
> ToleranceTables	0	1			✓	✓
>> ToleranceTable	0	∞		Additional items provided from Vision to expand the features of Tolerance Tables with AutoSetup capabilities	✓	✓
>>> ReferencedToleranceTableNumber	1	1	int	Refers to the tolerance table in RT Tolerance Table module	✓	✓
>>> ToleranceTableExtension	1	1			✓	✓
>>>> GantryRtnSetup	0	1	string	Setup attributes may have following type: Automatic Manual Remote	✓	✓
>>>> CollRtnSetup	0	1	string		✓	✓
>>>> CollXSetup	0	1	string		✓	✓
>>>> CollYSetup	0	1	string		✓	✓
>>>> PatientSupportAngleSetup	0	1	string		✓	✓
>>>> CouchLngSetup	0	1	string		✓	✓
>>>> CouchVrtSetup	0	1	string		✓	✓
>>>> CouchLatSetup	0	1	string		✓	✓
>>>> TableTopEccentricAngleSetup	0	1	string		✓	✓
> DoseReferences	0	1			✓	✓
>> DoseReference	0	∞			✓	✓
>>> ReferencedDoseReferenceNumber	1	1	int	Reference to the identification number of the Dose Reference (300A,0012) in the RT Prescription module which is a representation of our reference point	✓	✓
>>> DoseReferenceExtension	1	1		Additional items provided from Vision to expand the features of reference points.	✓	✓
>>>> DailyDoseLimit	0	1	decimal	Unit is [Gy]	✓	✓
>>>> SessionDoseLimit	0	1	decimal	Unit is [Gy]	✓	✓
>>>> Breakpoints	0	1			✓	✓
>>>>> Breakpoint	0	∞		Breakpoint extension since DICOM has just one DeliveryWarningDose without a description.	✓	✓
>>>>>> BreakpointDose	1	1	decimal	Unit is [Gy]	✓	✓
>>>>>> BreakpointWarning	1	1	string	Text which describes the breakpoint. Max length is 254 characters	✓	✓

Table 27: RT Plan Extended Interface XML Structure

D.2 RT Beams Treatment Record

The XML data structure for RT Beams Session Record IOD is contained in RT Beams Session Record Module in private Treatment Session Beam Data Attribute with tag (3261,102A).

The structure of the XML data structure is described in the following table.

Column “Operational Mode” indicates the presence for certain XML nodes depending of the applications Operational Mode

Legend for column “Operational Mode”:

✓ Attribute supported

✗ Attribute not supported

Attributes not supported anymore in the Extended Interface XML data are covered by standard DICOM attributes.

Node Name	Occurrence		Data Type	Node Description	Operational Mode	
	Min	Max			VMS Console System 6.5	VMS Console System 8.8 / QA
RTBeamSessionRecordExtendedIF	0	1			✓	✓
> DoseOverrides	0	1			✓	✓
>> DoseOverride	0	∞		There may be as many DoseOverride nodes as Reference Points.	✓	✓
>>> DoseOverrideType	1	1	string	Type of dose overrides. Supported are: BREAKPOINT: Breakpoint dose limit overridden DAILYDOSE: Daily dose limit overridden SESSIONDOSE: Session dose limit overridden TOTALDOSE:	✓	✓
>>> Dose	0	1	decimal	Contains the specific overridden/authorized dose for DoseOverrideType 'BREAKPOINT' at the Reference Point referenced by Dose Reference Number. Unit is [Gy]	✓	✓
>>> DoseReferenceNumber	1	1	non-negative int	References the Reference Point on which the dose was applied.	✓	✓
>>> OperatorsName	1	1		Operator Name who overrode/approved the specific doses.	✓	✓
>>>> FamilyName	0	1	string	Max length is 64 characters.	✓	✓
>>>> GivenName	0	1	string	Max length is 64 characters	✓	✓
>>>> MiddleName	0	1	string	Max length is 64 characters	✓	✓
>>>> Prefix	0	1	string	Max length is 64 characters	✓	✓
>>>> Suffix	0	1	string	Max length is 64 characters	✓	✓

Extended Interface, Extended Interface – Private

> TraySpecifications	0	1			✓	✗
>> TraySpecification	1	∞		As many nodes as tray applied for the treated beam.	✓	✗
>>> TrayID	1	1	string	That's the parameter which needs to be defined when a tray is defined/acquired. Max length is 16 characters	✓	✗
>>> SourceTrayDistance	0	1	int	Radiation Source to attachment edge of tray assembly (mm).	✓	✗
> AdditionalOperators	0	1			✓	✓
>> OperatorsName	1	2		If the 'Show Sign Off Dialog' is checked in ITAdmin -> MachineConfiguration -> Preferences, the Sign Off Dialog will be shown after closing the patient. Three OperatorsName may be entered in this dialog. The first OperatorsName will be sent through the standard attribute Operator Name (0008,1070) in the RT Beams Session Record module, the remaining two names if available will be sent here in the Extended Interface	✓	✓
>>> FamilyName	0	1	string	Max length is 64 characters.	✓	✓
>>> GivenName	0	1	string	Max length is 64 characters	✓	✓
>>> MiddleName	0	1	string	Max length is 64 characters	✓	✓
>>> Prefix	0	1	string	Max length is 64 characters	✓	✓
>>> Suffix	0	1	string	Max length is 64 characters	✓	✓

Table 28: RT Beams Treatment Record Extended Interface XML Structure

Extended Interface, Extended Interface – Private